



Analytical Balances

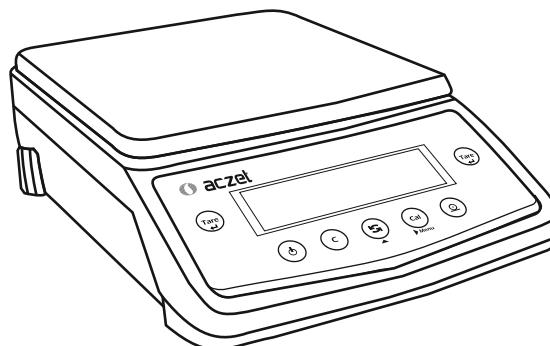

Carat Balances

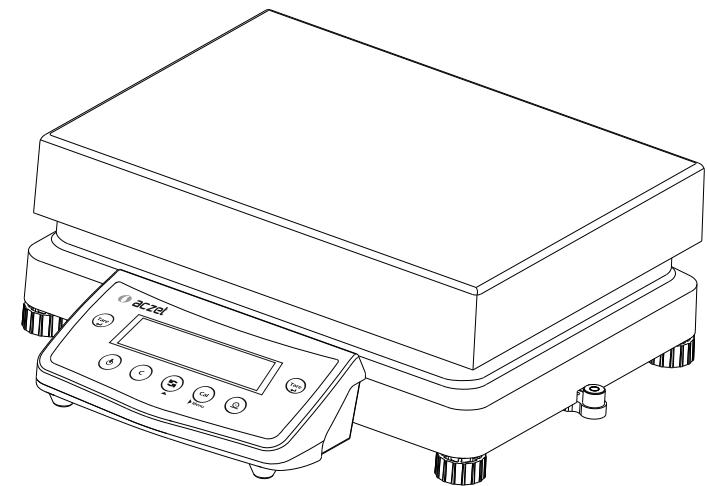

Precision Balances

High Precision Industrial Balances

# C Y - S E R I E S M A N U A L

## Contents

|          |  |           |
|----------|--|-----------|
| <b>1</b> | <b>Introduction</b>                      | <b>4</b>  |
| 1.1      | Warning & Safety Precautions             | 5         |
| 1.2      | Getting Started                          | 6         |
| 1.3      | Layout                                   | 7         |
| <b>2</b> | <b>Setting up the Balance</b>            | <b>10</b> |
| 2.1      | Location                                 | 13        |
| 2.2      | Warm up                                  | 15        |
| 2.3      | Keys of Balance                          | 16        |
| <b>3</b> | <b>Power On</b>                          | <b>18</b> |
| <b>4</b> | <b>Simple Weighing</b>                   | <b>20</b> |
| 4.1      | External Calibration                     | 24        |
| 4.2      | Internal Calibration                     | 27        |
| 4.3      | Calibration Test                         | 30        |
| 4.4      | Calibration Test with Actual Calibration | 32        |
| <b>5</b> | <b>Overview of Menu</b>                  | <b>35</b> |
| 5.1      | Operating Instruction                    | 36        |
| 5.2      | Description of Menu                      | 37        |
| <b>6</b> | <b>Functions</b>                         | <b>47</b> |
| 6.1      | Piece Counting                           | 47        |
| 6.2      | Percent Weighing (%)                     | 52        |
| 6.3      | Custom Units                             | 59        |
| 6.4      | Animal Weighing                          | 63        |
| 6.5      | Formulation                              | 67        |
| 6.6      | Check weighing                           | 71        |

|           |   |            |
|-----------|---|------------|
| 6.7       | Totalization .....                              | 75         |
| 6.8       | Density Determination .....                     | 79         |
| 6.9       | Pipette Calibration .....                       | 85         |
| 6.10      | Statistics .....                                | 92         |
| <b>7</b>  | <b>Parameter Settings .....</b>                 | <b>96</b>  |
| 7.1       | Time & Date Settings .....                      | 99         |
| 7.2       | BATCH ID / SAMPLE ID / TEXT3 DATA Setting ..... | 101        |
| 7.3       | Customize Print Setting .....                   | 102        |
| 7.4       | Auto Calibration .....                          | 104        |
| 7.5       | Windows Direct Communication .....              | 107        |
| <b>8</b>  | <b>ISO / GLP - Compliant Printout .....</b>     | <b>110</b> |
| <b>9</b>  | <b>Data Interface113 .....</b>                  | <b>113</b> |
| 9.1       | Data Output Format With 26 Characters .....     | 114        |
| 9.2       | Data Input Format .....                         | 116        |
| 9.3       | Cabling Diagram .....                           | 117        |
| <b>10</b> | <b>Error Codes .....</b>                        | <b>118</b> |
| <b>11</b> | <b>Care &amp; Maintenance .....</b>             | <b>120</b> |
| <b>12</b> | <b>Dimensional Drawings .....</b>               | <b>124</b> |
| <b>13</b> | <b>Specification .....</b>                      | <b>128</b> |
| <b>14</b> | <b>Accessories .....</b>                        | <b>140</b> |

## 1. Introduction

The models of the CY Series (0.1mg, 1mg, 10mg, 100mg & 0.001ct) are weighing instruments of special and high accuracy designed for the measurement of mass, covering a range from 0.01mg to 100 kg.

CY Series models meet the highest requirements on the accuracy and reliability of weighing results through the following features:

- Filtering for unfavorable ambient conditions, such as vibration, drafts, etc.
- Stable and repeatable weighing results
- Excellent readability under any lighting conditions
- Rugged, durable weighing system

These weighing instruments speed up your simple routine applications through following features:

- Extremely fast response times
- Built-in applications
  - Counting
  - Percent weighing
  - Animal weighing
  - Formulation
  - Totalization
  - Custom Unit
  - Check Weighing
  - Density Determination
  - Pipette Calibration
  - Statistics
- Total ease of operation
- Direct Communication with MS Excel, MS Word and other windows application.
- ISO/GLP-compliant recording capability for printouts
- Serial RS-232 and USB interface to PC or Printer

## 1.1 Warnings and Safety precautions

The balance has been constructed in accordance with the European Directives as well as international regulations and standards for operation of electrical equipment, electromagnetic compatibility, and stipulated safety requirements. Improper use or handling, however, can result in damage and/or injury.

To prevent damage to the equipment, please read these operating instructions carefully before using your balance.

Keep these instructions in a safe place. Follow the instructions below to ensure safe and trouble-free operation of your balance.

- ⚠ Do not use this balance/scale in a hazardous area/location.
- ⚠ If you use electrical equipment in installations and under ambient conditions requiring higher safety standards, you must comply with the provisions as specified in the applicable regulations for installation in your country.

- ⚠ Make sure that the voltage rating printed on the AC adapter is identical to your local line voltage.
- ⚠ Warning when using pre-wired RS-232 connecting cables: The pin assignments in RS-232 cables purchased from other manufacturers may be incompatible with Aczet balances. Be sure to check the pin assignment against the chart on page 117 before connecting the cable.
- The only way to switch the power off completely is to disconnect the AC adapter.
- Connect only Aczet accessories and options, as these are optimally designed for use with your Aczet balances.
- Note on Installation: The operator shall be responsible for any modifications to Aczet equipment **and for** any connections of cables or equipment not supplied

by Aczet and must check and, if necessary, correct these modifications and connections. On request, Aczet will provide information on the minimum operating specifications

- Protect the DC adapter and the weighing instrument from contact with liquids.
- When cleaning your balance, make sure that no liquid enters the balance housing; use only a slightly moistened cloth to clean the balance.
- Do not open the balance/scale housing. If the seal is broken, this will result in forfeiture of all claims under the manufacturer's warranty.
- If you have any problems with your balance contact your local Aczet office, dealer or service center

## 1.2 Getting Started

### Storage and Shipping Conditions

Do not expose the balance/scale to extreme temperatures, blows, shocks, vibration or moisture.

### Unpacking the Equipment

After unpacking the balance/scale, check it immediately for any visible damage as a result of rough handling during shipment

If you see any sign of damage:  
Contact your local Aczet office,  
dealer or service center

It is a good idea to save the box and all parts of the packaging until you have successfully installed your balance.  
Only the original packaging provides the best protection for shipment.  
Before packing your balance, unplug all connected cables to prevent damage.

### Accessories Supplied

The equipment supplied includes the following :

- Balance with display and control unit
- Operating Manual
- DC adapter
- Gem bowl [CY (0.001ct)]
- Pan Support [CY(0.1mg, 1mg, 0.001ct)]
- Weighing pan
- Draft shield [CY(0.1mg, 1mg, 0.001ct)]
- Wind Shield [CY(0.1mg, 1mg, 0.001ct)]
- Base Plat S.S. [CY(0.1mg, 1mg, 0.001ct)]
- Pan Cover [CY(0.1mg, 0.001ct)]
- 1 Pair of Corner hole Cover [CY(0.1mg, 1mg, 0.001ct)]


### Cautionary notes

Aczet balances may not be operated in hazardous areas.




Before attachment of the DC adapter, check whether the imprinted voltage value matches the local supply voltage. If it does not, contact your local ACZET dealers.

ACZET balance may only be used indoor in dry environment.

### CY (0.1 mg & 0.001ct)

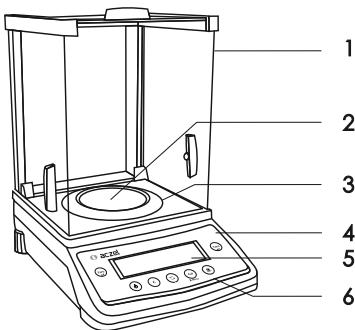

### CY (1 mg)

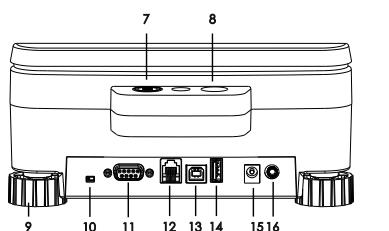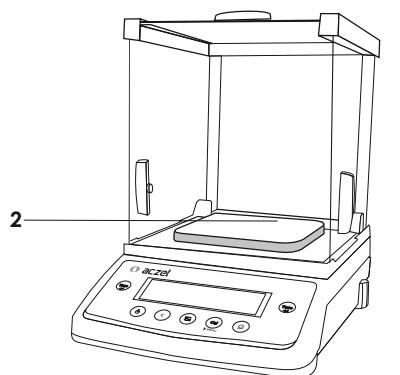

## 1.3 Layout


### CY (0.1mg, 1mg & 0.001ct)

1. Draft shield [CY(0.1mg, 1mg & 0.001ct)]
2. Weighing Pan (90Ømm)
3. Pan Cover
4. Model Plate
5. Display
6. Keypad
7. Sprit Level
8. Provision for anti-theft device
9. Leveling feet
10. Calibration Switch (for Verified Balance)
11. RS 232C interface
12. Additional Display Socket(RJ-45)
13. USB Port-B
14. USB Port-A
15. DC adapter socket
16. Foot Tare Switch Socket.
17. Gem Bowl (CY - 0.001ct)

### CY (1mg with Draft shield)

1. Draft shield [CY(0.1mg, 1mg & 0.001ct)]
2. Weighing Pan ( 128mm x 128mm )
4. Model Plate
5. Display
6. Keypad
7. Sprit Level
8. Provision for anti-theft device
9. Leveling feet
10. Calibration Switch (for Verified Balance)
11. RS 232C interface
12. Additional Display Socket(RJ-45)
13. USB Port-B
14. USB Port-A
15. DC adapter socket
16. Foot Tare Switch Socket.

**Note :** Keys, operation and display are identical for all ACZET balances.

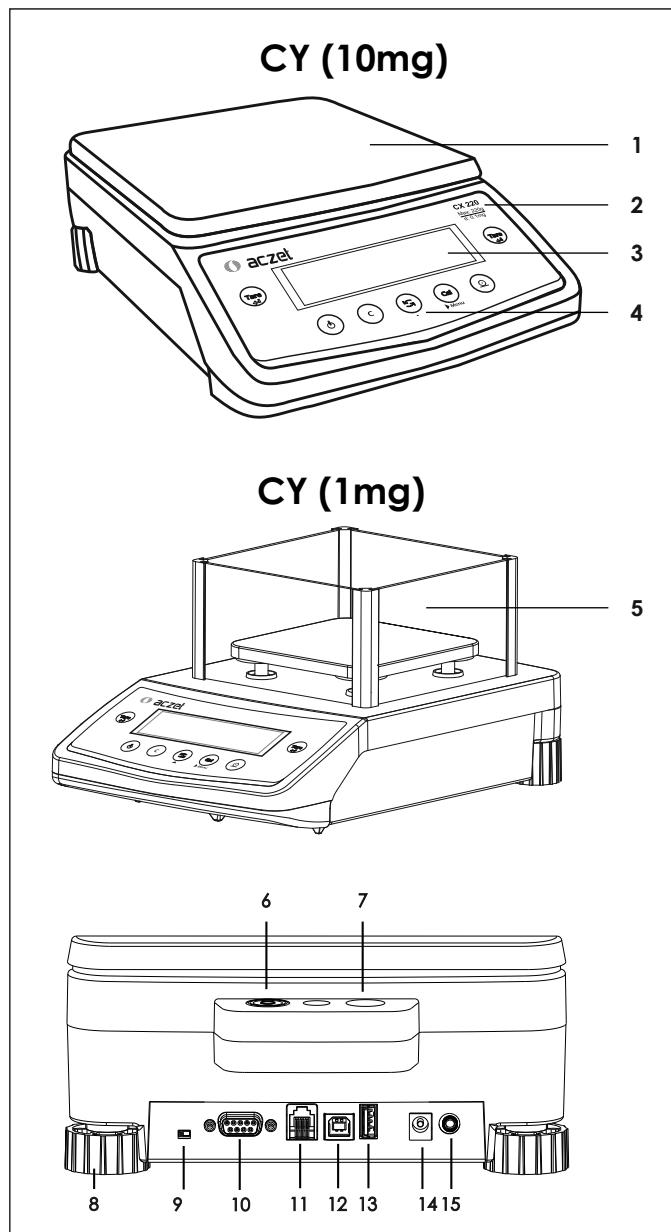


### CY (10mg)

1. Weighing pan (198 mmX 205 mm)
2. Model plate
3. Display
4. Keypad
6. Spirit Level
7. Provision for anti-theft device
8. Leveling feet
9. Calibration Switch (for Verified Balance)
10. RS232C interface
11. Additional Display Socket(RJ-45)
12. USB Port-B
13. USB Port-A
14. DC adapter socket
15. Foot Tare Switch Socket.

### CY (1mg with wind shield)

1. Weighing Pan (128mm x 128mm)
2. Model Plate
3. Display
4. Keypad
5. Draft shield [CY(0.1mg, 1mg & 0 .001ct)]
6. Sprit Level
7. Prevision for anti-theft device
8. Leveling feet
9. Calibration Switch (for Verified Balance)
10. RS 232C interface
11. Additional Display Socket(RJ-45)
12. USB Port-B
13. USB Port-A
14. DC adapter socket
15. Foot Tare Switch Socket.

**Note :** Keys, operation and display are identical for all ACZET balances.

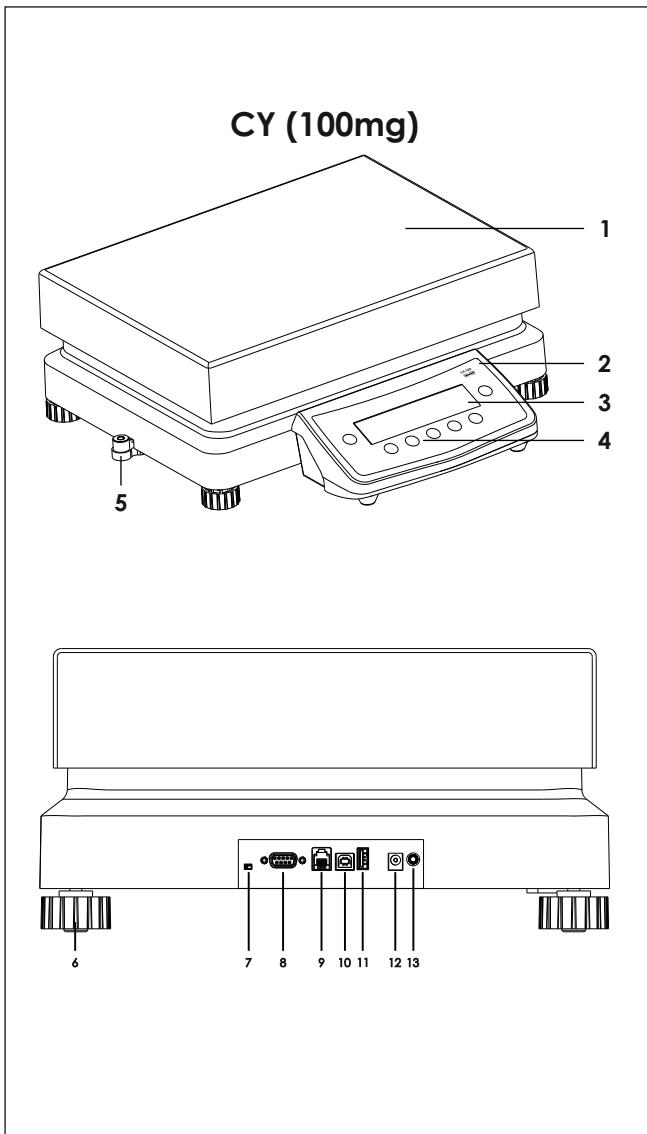


### CY (100mg)

1. Weighing pan (400mm x 300mm)
2. Model plate
3. Display
4. Keypad
5. Spirit Level
6. Leveling feet
7. Calibration Switch (for Verified Balance)
8. RS232C interface
9. Additional Display Socket(RJ-45)
10. USB Port-B
11. USB Port-A
12. DC adapter socket
13. Foot Tare Switch Socket.

**Note :** Keys, operation and display are identical for all ACZET balances.

## 2. Setting Up the balance

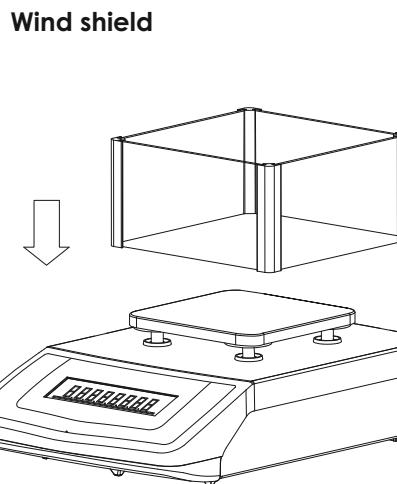


### Balance with Wind Shield Chamber

- Position the Wind shield carefully on the balance.


**Step 1:** Open your New balance and Wind shield.

**Step 2:** Place the Bushes in respective slots on the top body of the balance. Carefully place the weighing pan on the bushes. now place the Wind Shield over the pan such that it does not touch the weighing pan.


**Note :** Ensure there must be gap between the pan and the Wind Shield .

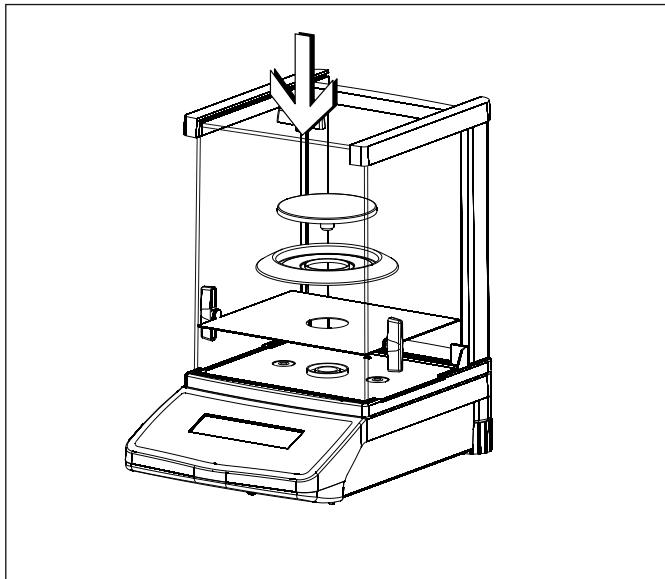


- Place the components listed below inside the chamber in the order given:  
**(For CY (0.1mg & 0.001ct) Series Balances)**
- Corner Cover
- Base plate
- Pan Cover
- Weighing pan

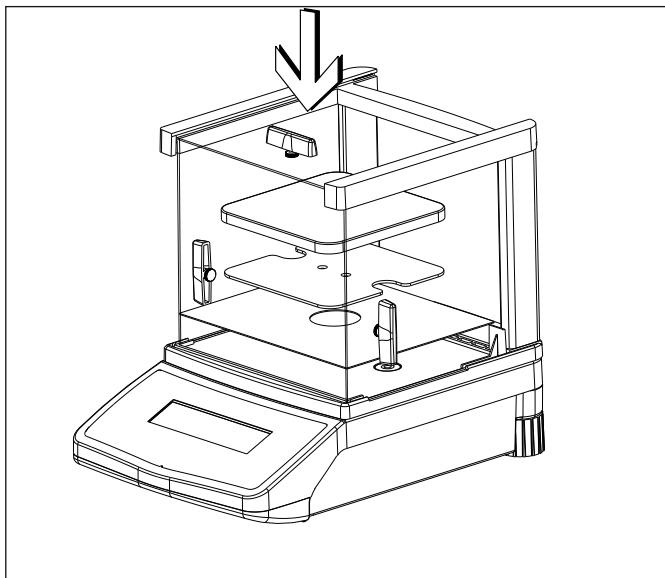

- Place the components listed below inside the chamber in the order given:  
**(For CY (1mg) Series Balances)**
- Corner Cover
- Base plate
- Pan Support
- Weighing pan

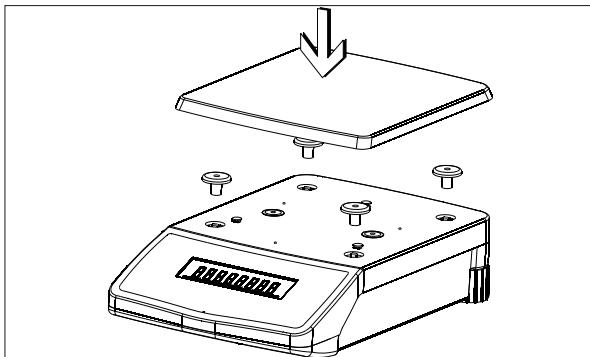

- Place the components listed below inside the chamber in the order given:  
**(For CY (10mg) Series Balance)**
- Bush
- Weighing pan

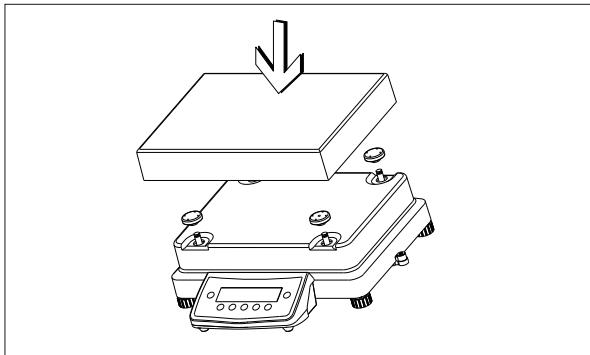


- **Balances with a Rectangular Weighing Pan and a Weighing Capacity over 10 kg**
- Place the weighing pan on the balance/scale


### **Under Weighing**

A port for a under weighing hanger is located on the bottom of the balance.

- Remove the under weighing cover from the bottom of the balance (as shown alongside)
- Suspend the below-balance weighing hook supplied from the hanger
- If necessary, install a shield for protection against drafts

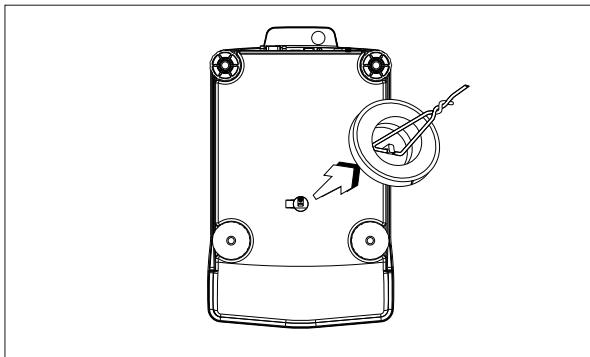

## 2.1 Location

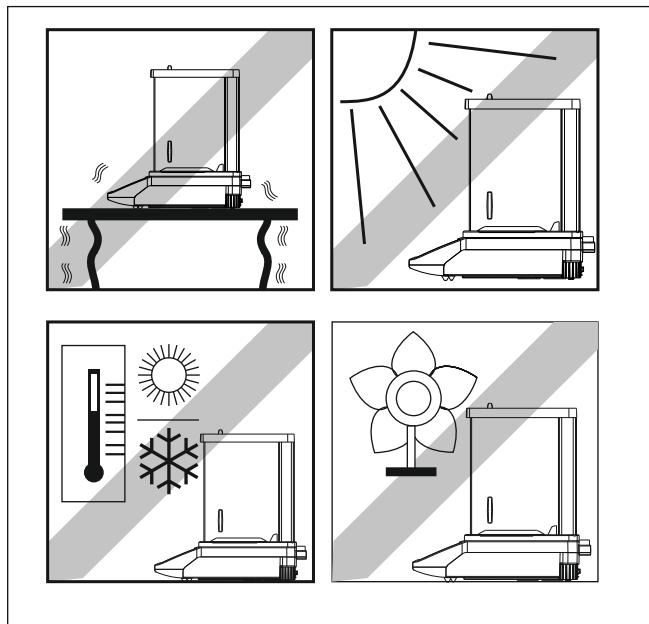

### The optimum location


The correct location makes an important contribution to the accuracy of the weighing results of high-resolution analytical and precision balances.

Hence, ensure a stable, vibration-free position as horizontal as possible.

### Avoid

- Direct sunlight
- Excessive temperature fluctuations,
- Drafts (Power ----- Air Conditioning System, Fans can also cause drafts)


The best position is an a stable bench in a corner protected against drafts as far possible from doors, windows, radiators or the ventilation slots of air conditioners.

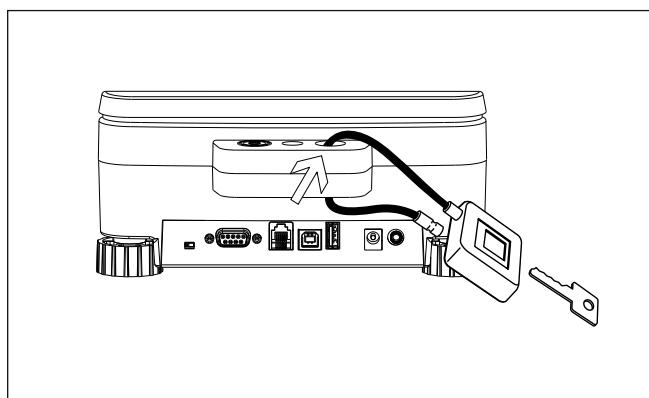

### Anti-theft device

Aczet Balance are equipped with a lug for optional anti-theft device.

The anti-theft device (cable with lock) is suitable for all models. It is available from ACZET under order number CAD01.

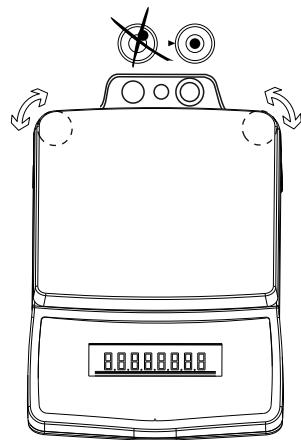


## Leveling the Balance

Aczet balances have a level control and adjustable leveling feet to compensate for slight irregularities in the weighing bench surface. The balance is exactly horizontal when the air bubble is in middle.

### Leveling Balances with a Weighing Capacity up to 10 kg

Turn the two leveling feet as desire picture in diagram so that air bubble comes in middle.

|               |              |  |
|---------------|--------------|--|
| Air bubble at | "12 o'clock" | Turn both leveling feet counter-clockwise.                                 |
| Air bubble at | "3 o'clock"  | Turn left leveling foot clockwise,<br>right leveling foot counterclockwise |
| Air bubble at | "6 o'clock"  | Turn both leveling feet clockwise  |
| Air bubble at | "9 o'clock"  | Turn left leveling foot clockwise,<br>right leveling foot counterclockwise |

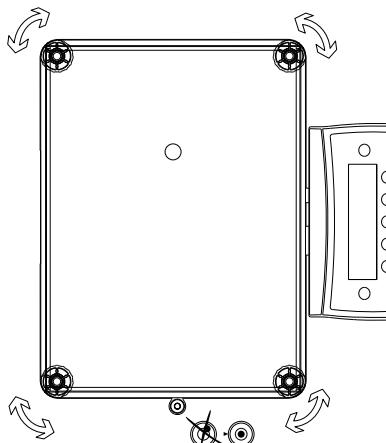


### Leveling Balances with a Weighing Capacity over 10 kg

- Adjust the leveling feet until the air bubble is centered within the circle of the level indicator

**Note :** The balance must be re-leveled each time it is moved to a new location.

## 2.2 Warm Up

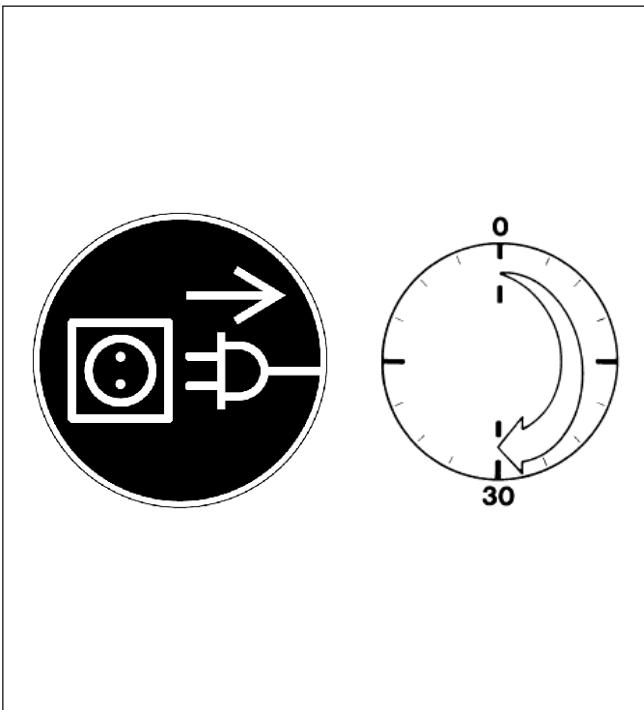

### Connecting Electronic Peripheral Devices

Make absolutely sure to unplug the balance from DC power before you connect or disconnect a peripheral device (printer or PC) to or from the interface port.


### Warmup Time

To deliver exact results, balance must warm up to operating temperature for as leasted below the first weighing operation is carried out.

- CY (0.1mg) / CY (0.001ct) all Analytical models: at least 60 minutes
- CY (1mg) / CY (10mg) / CY (100mg) all Precision models: at least 30 minutes

Using Verified Balances as Legal Measuring Instruments in the EU\* balance must warm up for at least 24 hours after initial connection to DC power.

## 2.3 Keys of Balance

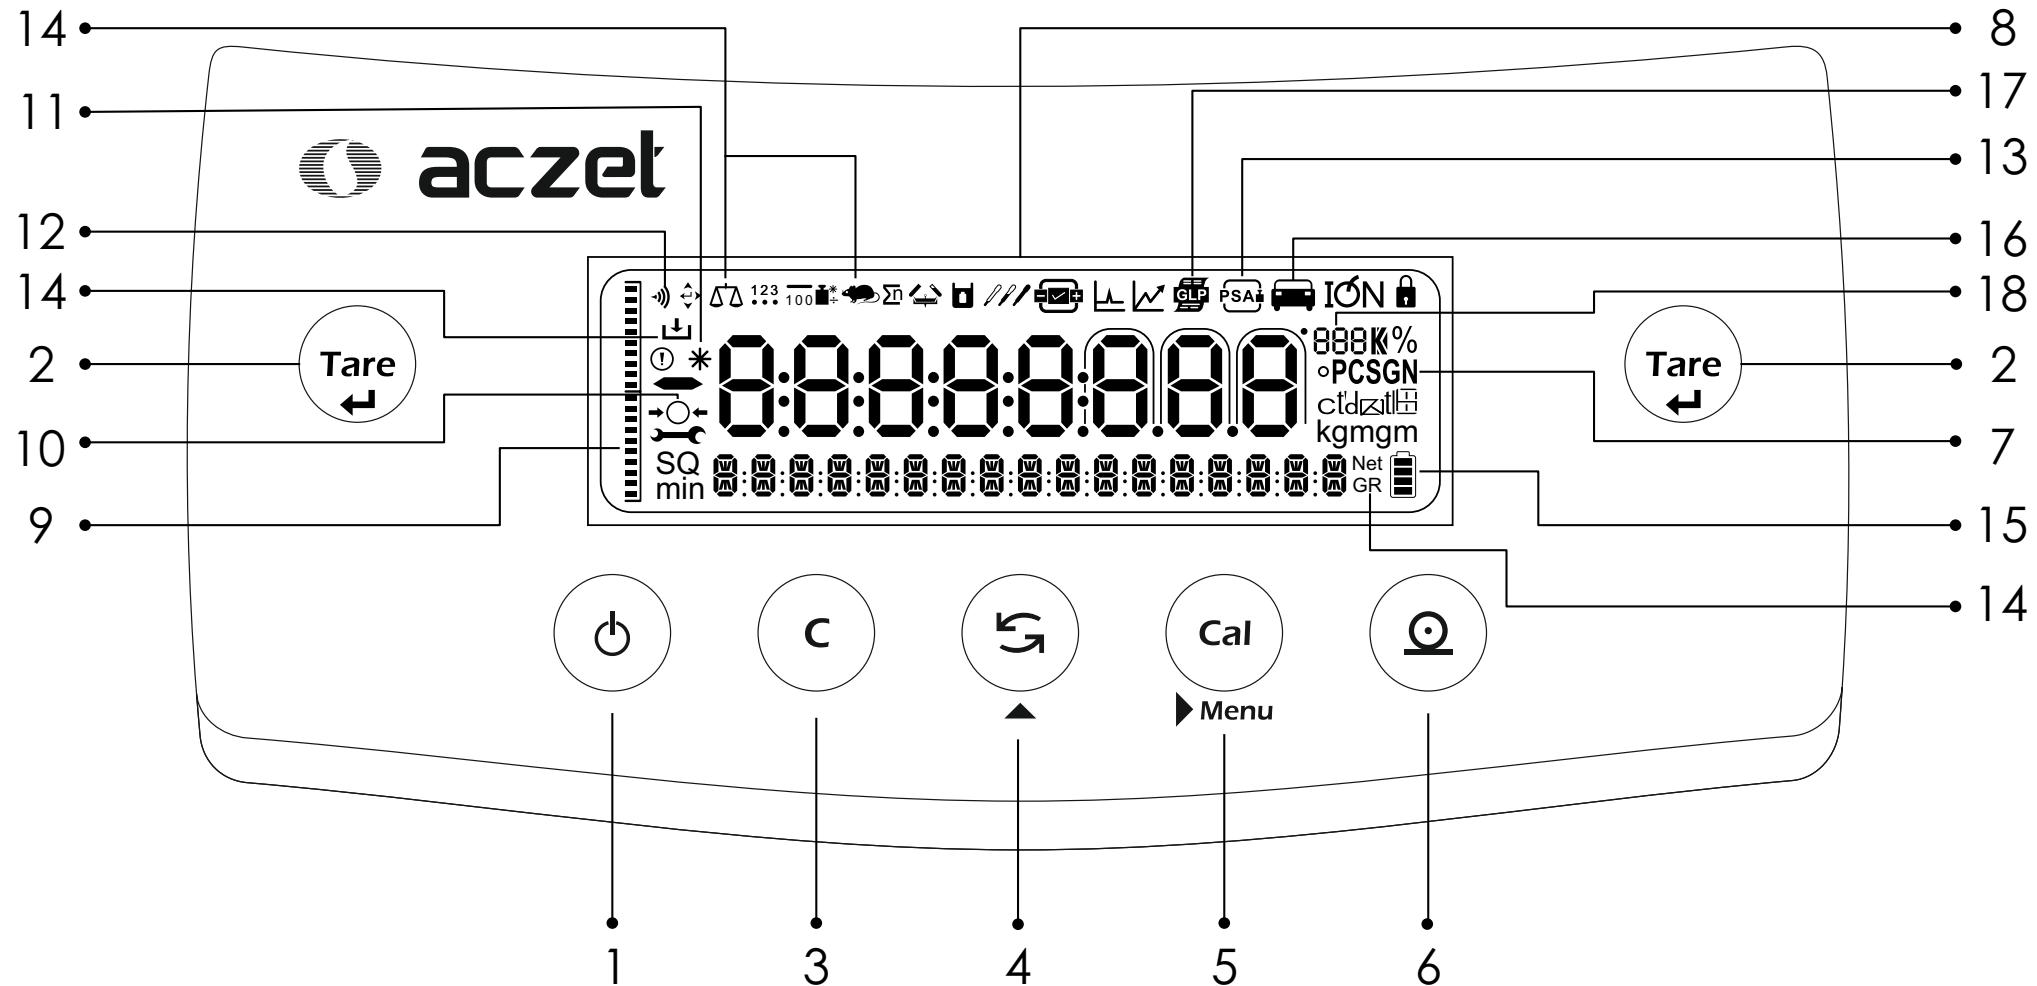

|   |   |    |  |
|---|---|----|--|
| 1 | On/Off key: Switches the display on / off   | 9  | Capacity Bar : This indicates the total amount of weight on the Pan                            |
| 2 | Tare key: Press here to tare the weight of any container so that the readout shows the net weight of samples, also used to store reference settings. This key used to delete the statistics when F StAt mode.                         | 10 | Stability Symbol : This symbol is displayed when the weight place on the pan achieve stability |
| 3 | Cancel Function : Delete (Clear Function) This key is generally used to interrupt/cancel functions; for example: – to end an application program<br>– to interrupt calibration/ adjustment routines                                   | 11 | Asterik Symbol : This Symbol is displayed when the display is locked                           |
| 4 | Toggle Key : Press here to change the Unit, Also used to increment digit.   | 12 | Stability Filer : This symbol indicates the chosen stability filter                            |
| 5 | Cal Menu Function : Press here to start calibration/ adjustment or to enter user menu, Also use to shift flashing digit from left to right. this key is used in the F PiP mode to accept the volume during the calibration procedure. | 13 | Symbol indicating that the Auto / Manual calibration/adjustment function is active             |
| 6 | Print Key : Press this key to send displayed values over the built-in data interface to a DataPrint printer or a PC.  | 14 | Symbol indicating the active program   |
| 7 | Weight Units  | 15 | Battery Level Indicator : This symbol is indicates the Current charge of the battery           |
| 8 | Weight readout in the selected weight unit  | 16 | Symbol indicating that a printout is being generated   |
|   |   | 17 | Symbol indicating that a GLP compliant printout is being generated                             |
|   |   | 18 | Seven segment readout indicating the active program  |


### 3. Power ON

Connect DC Adaptor and Power ON the balance.



- It will display version number for software
- It will display numeric countdown
- It will display 88888888
- The system initialization process will begin with the display indicating the current progress. (INIT 1% to INIT 100%)
- After the initialization is complete (100%) It will enter stand by mode & display clock.

#### Stand by Mode

- After Power ON and initial test balance will automatically come in stand by mode.
- Press ON / OFF key to come to basic weighing
- Press ON / OFF key in basic weighing to come back to Stand by Mode

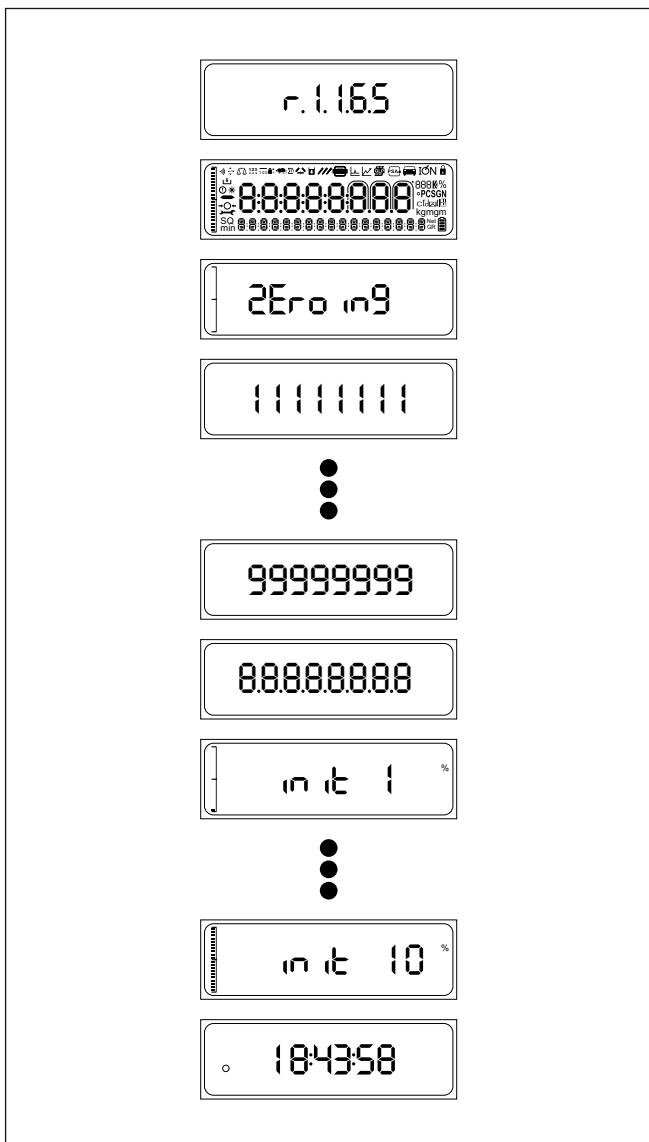

## Key Functionality in simple weighing mode

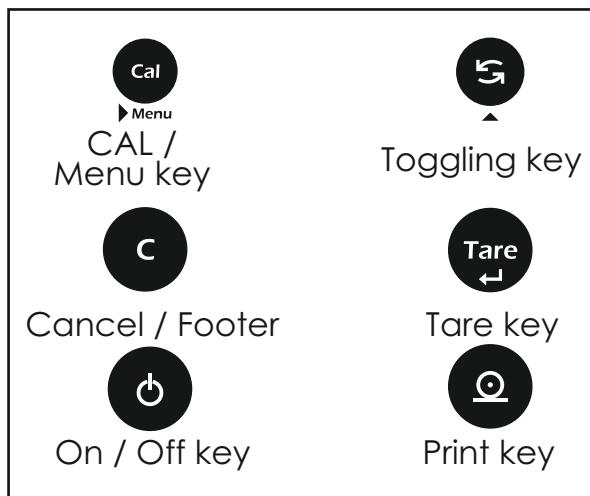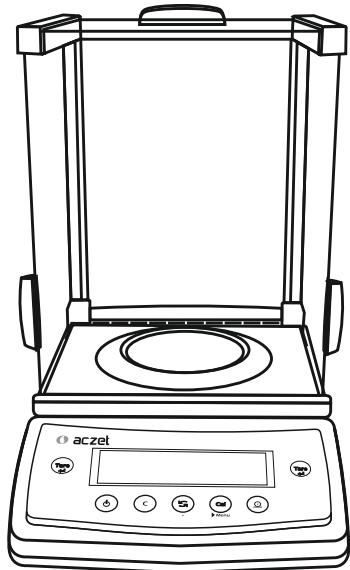

## Short-form operating Instructions

- ☞ Press key **briefly**
- ☞ Press and **hold** key until desired display appears
- ▼ Automatic procedure

Aczet balances have several control levels the following section explains key functionality in simple weighing mode.

| Weighing mode (operation)                  |                                     |
|--|-------------------------------------|
| Press briefly ☞                            | Press & Hold ☞                      |
| ● Switch on & off                          |                                     |
| ● Switch References                        |                                     |
| ● Change Weighing Unit                     |                                     |
|  | ● Calibrate (adjust)<br>● Call Menu |
| ● Print Weighing Results                   |                                     |
| ● Tare ↕<br>● Confirm Setting              | ● Confirm Reference Setting         |
| ● Abort / Cancel and Footer when GLP is ON |                                     |


## 4. Simple Weighing

### Purpose

The basic weighing function is always accessible and can be used alone or in combination with an application program (counting, weighing in percent, etc.).


### Features

- Taring the balance you can tare the balance within the entire weighing range.
- Assigning IDs to weights (as needed)
- Printing weights

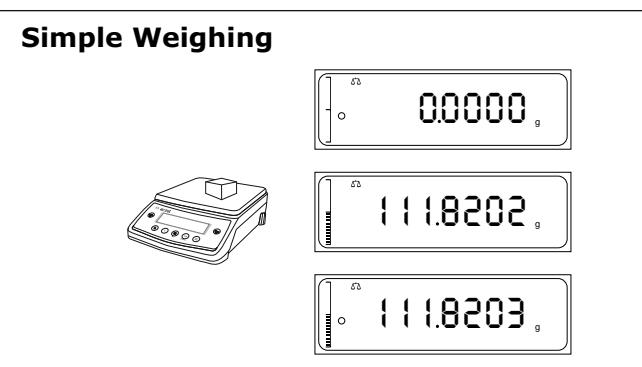

### 4.0.1 Simple weighing


- ⇒ Place weighing sample on the weighing pan.
- ⇒ Wait until the stability symbol appears
- ⇒ Read the result.
- ⇒ Bar Graph will glow according to weight kept ON the PAN.

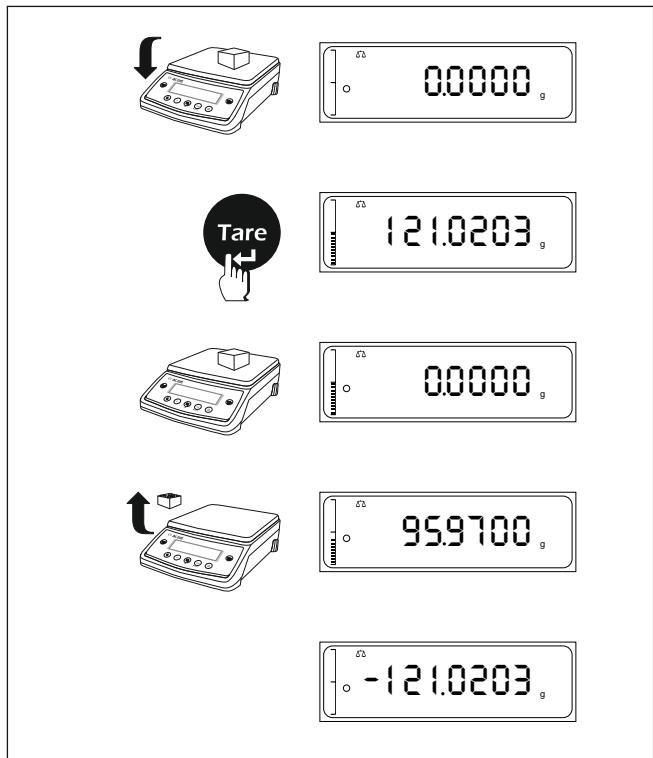

#### 4.0.2 Taring

- ⇒ Place empty container on the balance.
- ⇒ The weight is displayed.
- ⇒ Press <Tare> key briefly, the balance displays zero
- ⇒ Add weighing sample to container, the net weight is displayed.

If the container is removed from the balance, the tare weight will be shown as a negative value.

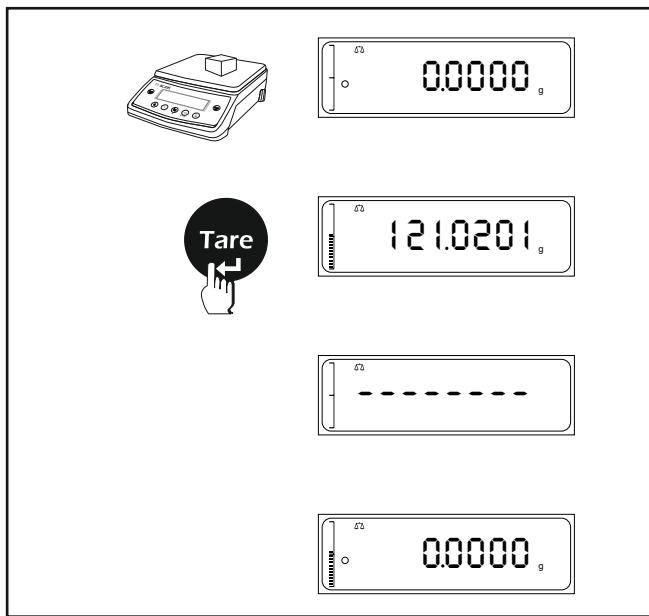

In case if stability is not achieved & user presses <TARE> key, display will shows “-----” until stability is achieved.

Display then shows “0.0000 gm”

#### 4.0.3 Switching of weight units

All Aczet balances can display weight values in different weight units.

The **factory setting** is Unit 1 (gm), Unit 2 (ct), Unit 3 (gm)

##### Switching between unit 1, unit 2 and unit 3

- ⇒ Press <TOGGLE> key the display switches to the 2nd weight unit.
- ⇒ Press <TOGGLE> key again, the display switches to the 3rd weight unit. OR Application unit (If same is selected in menu)

**Note :** With **certified balances** the unit selection can be blocked following installation if required by national legislation.

#### 4.0.4 Simple weighing Print out

##### When Standard ON

Printouts generated when unit toggling is done between unit1 (g), Unit2 (ct), Unit3 (Oz) in Simple Weighing.

|   |             |
|---|-------------|
| + | 49.9999 g   |
| + | 249.9990 ct |
| + | 1.763690 oz |
| + | 49.9998 g   |
| + | 249.9990 ct |
| + | 1.763690 oz |
| + | 49.9999 g   |

##### When GLP ON

Printouts generated when unit toggling is done between unit1 (g), Unit2 (ct), Unit3 (Oz) in Simple Weighing.

|             |             |
|-------------|-------------|
| -----       | -----       |
| 05-Oct-23   | 10:35AM     |
|             | ACZET       |
| Model       | CY224C      |
| Ser.No.     | 12345678    |
| Ver.No.     | r.1.1.6.5   |
| Bal. ID.    | S/123       |
| -----       | -----       |
| Product :   | XYZ         |
| Batch ID :  | T123        |
| Sample ID : | L001        |
| +           | 49.9999 g   |
| +           | 249.9990 ct |
| +           | 1.763690 oz |
| +           | 49.9998 g   |
| +           | 249.9990 ct |
| +           | 1.763690 oz |
| +           | 49.9999 g   |
| -----       | -----       |
| 05-Oct-23   | 10:35AM     |
| Signature : | -----       |
| -----       | -----       |

##### When Customize ON


Printouts generated when unit toggling is done between unit1 (g), Unit2 (ct), Unit3 (Oz) in Simple Weighing.

|             |               |
|-------------|---------------|
| -----       | -----         |
| 05-Oct-23   | 10:35AM       |
|             | Aczet         |
|             | Mumbai, India |
| Model       | CY224C        |
| Ser.No.     | 12345678      |
| Ver.No.     | r.1.1.6.5     |
| Bal. ID.    | S/123         |
| -----       | -----         |
| Product :   | XYZ           |
| Batch ID :  | T123          |
| Sample ID : | L001          |
| +           | 49.9999 g     |
| +           | 249.9990 ct   |
| +           | 1.763690 oz   |
| +           | 49.9998 g     |
| -----       | -----         |
| 05-Oct-23   | 10:45AM       |
| Signature : | -----         |
| -----       | -----         |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.

## 4.1 External Calibration (Adjusting)

### Calibration

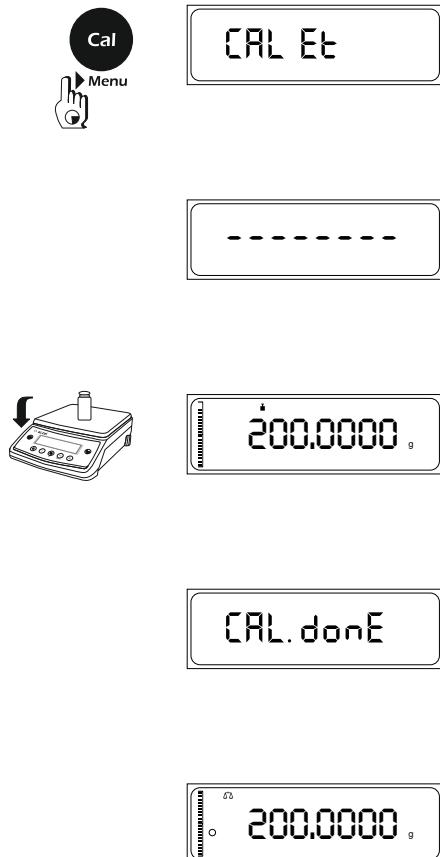

To obtain weighing results, the balance must be matched to the acceleration due to gravity at its location.

#### Calibration is necessary

- ⇒ Before the balance is used for the first time.
- ⇒ At regular intervals during weighing operation.
- ⇒ After a change in location.

#### Procedure

To obtain accurate results, the balance must be connected to the power supply and allowed to warm up to the operating temperature as described on Page No.15

Ensure that the weighing pan is unloaded and close the doors of the draft shield (if used). Balance should be Zero before calibration.

- ⇒ Have required calibration weight ready
- ⇒ Press and hold <CAL> key, display, shows "CAL Et"
- ⇒ Release <CAL> key now.
- ⇒ The required calibration weight value will be displayed.
- ⇒ Place calibration weight in center of pan.

The calibration (adjustment) is finished when "CAL donE" message is displayed. The balance is again in the weighing mode and ready for operation.

**Note :** With certified balances, the calibration can be disabled after installation if required by the national certification regulations.

The adjustment can be terminated at any time using the <CANCEL> key. The following message appears : 'Abort'

# External Calibration Report

If Balance is connected externally to PC or Data Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## Successful Calibration

### When Standard ON

|                   |           |
|-------------------|-----------|
| Calibration :     | External  |
| W-ID              | -----     |
| Temperature       | 32.898° C |
| Set +             | 20.00 g   |
| Diff.             | 0.00 g    |
| External Cal Done | -----     |
| Diff.             | 0.00 g    |

### When GLP ON

|                   |           |
|-------------------|-----------|
| 05-Oct-23         | 10:35AM   |
| ACZET             | -----     |
| Model             | CY224C    |
| Ser.No.           | 12345678  |
| Ver.No.           | r.1.1.6.5 |
| Bal. ID.          | S/123     |
| Product :         | XYZ       |
| Batch ID :        | T123      |
| Sample ID :       | L001      |
| Calibration :     | External  |
| W-ID              | -----     |
| Temperature       | 32.898° C |
| Set +             | 20.00 g   |
| Diff.             | 0.00 g    |
| External Cal Done | -----     |
| Diff.             | 0.00 g    |
| 05-Oct-23         | 10:35AM   |
| Signature :       | -----     |

### When Customize ON

|                   |               |
|-------------------|---------------|
| 05-Oct-23         | 10:35AM       |
| Aczet             | Mumbai, India |
| Model             | CY224C        |
| Ser.No.           | 12345678      |
| Ver.No.           | r.1.1.6.5     |
| Bal. ID.          | S/123         |
| Product :         | XYZ           |
| Batch ID :        | T123          |
| Sample ID :       | L001          |
| Calibration :     | External      |
| W-ID              | -----         |
| Temperature       | 32.898° C     |
| Set +             | 20.00 g       |
| Diff.             | 0.00 g        |
| External Cal Done | -----         |
| Diff.             | 0.00 g        |
| 05-Oct-23         | 10:35AM       |
| Signature :       | -----         |

# External Calibration Report

If Balance is connected externally to PC or Data Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## Unsuccessful Calibration

### When Standard ON

Calibration : External  
W-ID -----  
Temperature 32.898°C  
Set + 20.00 g  
External Cal Failed

### When GLP ON

05-Oct-23 10:35AM  
ACZET

Model CY224C  
Ser.No. 12345678  
Ver.No. r.1.1.6.5  
Bal. ID. S/123

Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : External  
W-ID -----  
Temperature 32.898°C  
Set + 20.00 g  
External Cal Failed

05-Oct-23 10:35AM  
Signature : -----

### When Customize ON


05-Oct-23 10:35AM  
Aczet Mumbai, India

Model CY224C  
Ser.No. 12345678  
Ver.No. r.1.1.6.5  
Bal. ID. S/123

Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : External  
W-ID -----  
Temperature 32.898°C  
Set + 20.00 g  
External Cal Failed

05-Oct-23 10:35AM  
Signature : -----

## 4.2 Internal Calibration

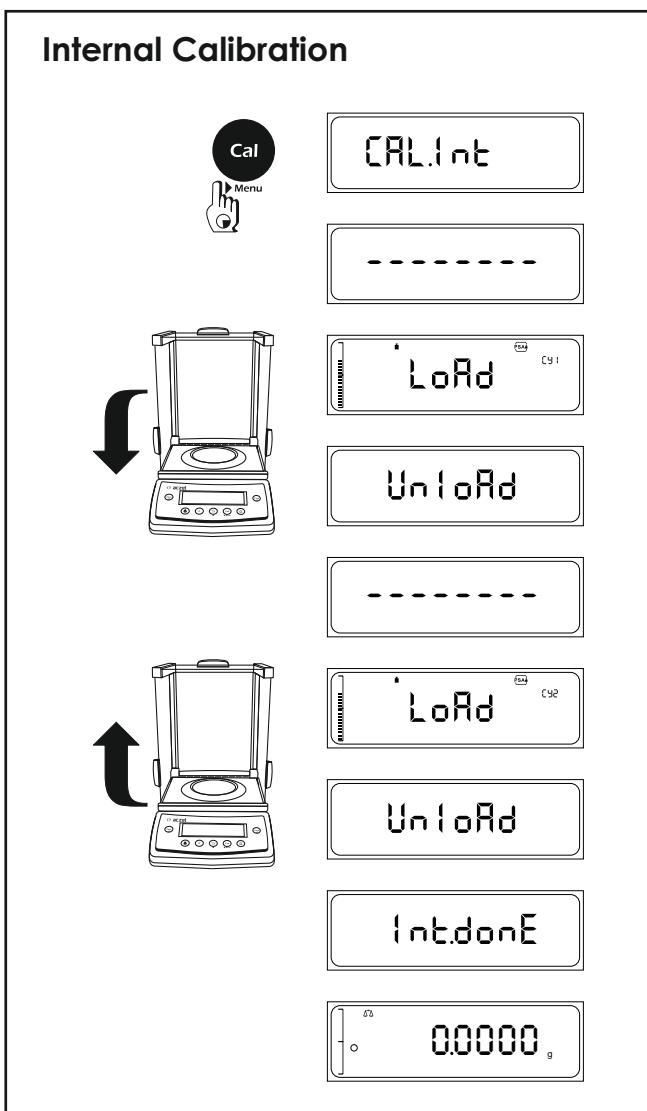

To obtain weighing results, the balance must be matched to the acceleration due to gravity at its location.

### Calibration is necessary

- ⇒ Before the balance is used for the first time.
- ⇒ At regular intervals during weighing operation.
- ⇒ After a change in location.

### Procedure

To obtain accurate results, the balance must be connected to the power supply and allowed to warm up to the operating temperature as described on Page No.15

Ensure that the weighing pan is unloaded and close the doors of the draft shield (if used). Balance should be Zero before calibration.

- ⇒ Press and hold **<CAL>** key, display, shows “CAL Int”
- ⇒ Release **<CAL>** key now.

Internal Calibration process Starts.....

- When the Internal Weight is being loaded “C” will be displayed on display.
- When the Internal Weight is being unloaded “CC” will be displayed on display.
- This cycle is performed twice.

Calibration is finished when ‘Int.done’ is message is displayed.

The adjustment can be terminated at any time using the **<CANCEL>** key. The following message appears : ‘Abort’

# Internal Calibration Report

If Balance is connected externally to PC or Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## Successful Calibration

### When Standard ON

|                   |          |
|-------------------|----------|
| Calibration :     | Internal |
| Start :           | Manual   |
| Temperature       | 29.449°C |
| Diff. +           | 0.0009 g |
| Internal Cal Done |          |
| Diff.             | 0.0000 g |

### When GLP ON

-----  
05-Oct-23 10:35AM

ACZET

|          |           |
|----------|-----------|
| Model    | CY224C    |
| Ser.No.  | 12345678  |
| Ver.No.  | r.1.1.6.5 |
| Bal. ID. | S/123     |

-----  
Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : Internal  
Start : Manual  
Temperature 29.449°C  
Diff. + 0.0009 g  
Internal Cal Done  
Diff. 0.0000 g

-----  
05-Oct-23 10:35AM

Signature : -----

### When Customize ON

-----  
05-Oct-23 10:35AM

Aczet  
Mumbai, India

|          |           |
|----------|-----------|
| Model    | CY224C    |
| Ser.No.  | 12345678  |
| Ver.No.  | r.1.1.6.5 |
| Bal. ID. | S/123     |

-----  
Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : Internal  
Start : Manual  
Temperature 29.449°C  
Diff. + 0.0009 g  
Internal Cal Done  
Diff. 0.0000 g

-----  
05-Oct-23 10:35AM

Signature : -----

# Internal Calibration Report

If Balance is connected externally to PC or Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## Unsuccessful Calibration

### When Standard ON

Calibration : Internal  
Start : Manual  
Temperature 29.495° C  
Internal Cal Failed

### When GLP ON

05-Oct-23 10:35AM  
ACZET

Model CY224C  
Ser.No. 12345678  
Ver.No. r.1.1.6.5  
Bal. ID. S/123

Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : Internal  
Start : Manual  
Temperature 29.495° C  
Internal Cal Failed

05-Oct-23 10:35AM  
Signature : -----

### When Customize ON

05-Oct-23 10:35AM  
Aczet  
Mumbai, India


Model CY224C  
Ser.No. 12345678  
Ver.No. r.1.1.6.5  
Bal. ID. S/123

Product : XYZ  
Batch ID : T123  
Sample ID : L001  
Calibration : Internal  
Start : Manual  
Temperature 29.495° C  
Internal Cal Failed

05-Oct-23 10:35AM  
Signature : -----

## 4.3 Calibration Test

### Calibration (adjusting)

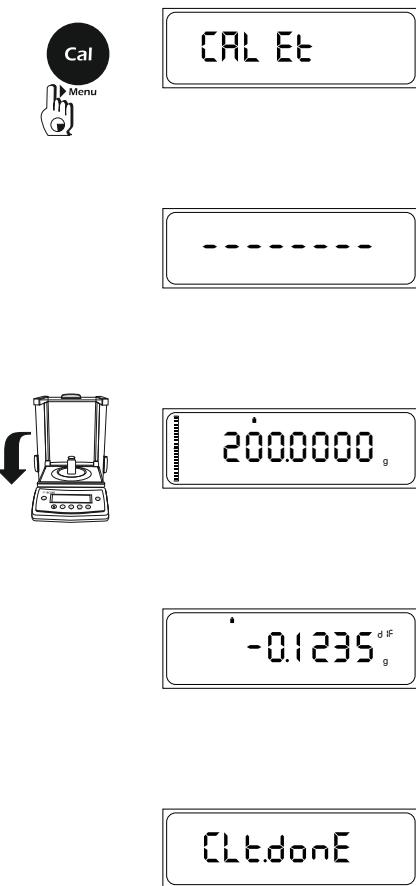

Calibration test determines the difference between the actual weight and the measured weight. Calibration test can be turned ON or OFF from the user menu. When ON, cal test would be performed on external or internal calibration whichever is selected in User Menu.

#### Procedure

- ⇒ Have required calibration weight ready
- ⇒ Press and hold <CAL> key, display, shows "CAL Et"
- ⇒ Release <CAL> key now.
- ⇒ The required calibration weight is shown on the display.
- ⇒ Place calibration weight in center of pan.
  
- ⇒ After the cal Test procedure is completed the difference between the actual & the measured weight will be displayed on display.

The adjustment can be terminated at any time using the <CANCEL> key. The following message appears : 'Abort'

# Calibration Test Report

If Balance is connected externally to PC or Data Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## When Standard ON

|                              |            |
|------------------------------|------------|
| Calibration :                | External   |
| W-ID                         | -----      |
| Temperature                  | 30.710°C   |
| Set +                        | 200.0000 g |
| Diff.                        | 0.0047 g   |
| <i>Calibration Test Done</i> |            |

## When GLP ON


|                              |            |
|------------------------------|------------|
| 05-Oct-23                    | 10:35AM    |
| ACZET                        |            |
| Model                        | CY224C     |
| Ser.No.                      | 12345678   |
| Ver.No.                      | r.1.1.6.5  |
| Bal. ID.                     | S/123      |
| -----                        |            |
| Product :                    | XYZ        |
| Batch ID :                   | T123       |
| Sample ID :                  | L001       |
| Calibration :                | External   |
| W-ID                         | -----      |
| Temperature                  | 30.710°C   |
| Set +                        | 200.0000 g |
| Diff. +                      | 0.0047 g   |
| <i>Calibration Test Done</i> |            |
| -----                        |            |
| 05-Oct-23                    | 10:35AM    |
| <i>Signature :</i> -----     |            |

## When Customize ON

|                              |            |
|------------------------------|------------|
| 05-Oct-23                    | 10:35AM    |
| Aczet                        |            |
| Mumbai, India                |            |
| Model                        | CY224C     |
| Ser.No.                      | 12345678   |
| Ver.No.                      | r.1.1.6.5  |
| Bal. ID.                     | S/123      |
| -----                        |            |
| Product :                    | XYZ        |
| Batch ID :                   | T123       |
| Sample ID :                  | L001       |
| Calibration :                | External   |
| W-ID                         | -----      |
| Temperature                  | 30.710°C   |
| Set +                        | 200.0000 g |
| Diff.                        | 0.0047 g   |
| <i>Calibration Test Done</i> |            |
| -----                        |            |
| 05-Oct-23                    | 10:35AM    |
| <i>Signature :</i> -----     |            |

## 4.4 Calibration Test with Actual Calibration

### Calibration (adjusting)

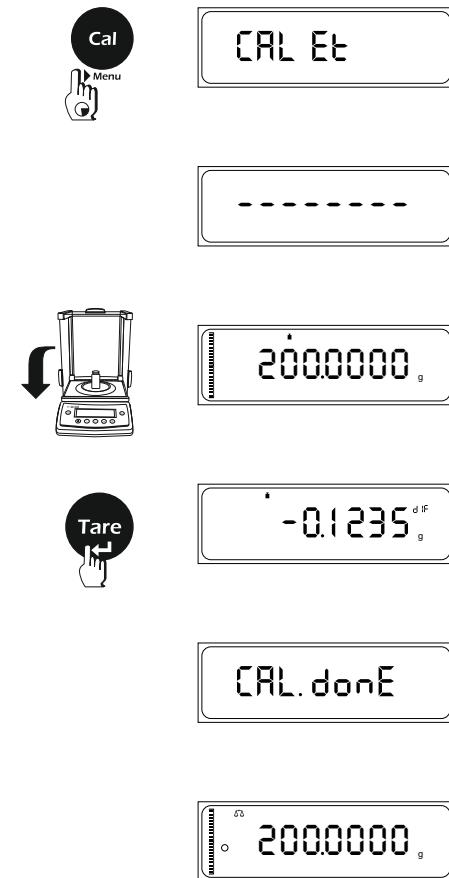

To correct the weighing results, the TARE key need to be pressed when the difference is display upon pressing the TARE key. Actual calibration is performed 'CAL done' is displayed and the weighing results are corrected as shown alongside.

#### Procedure

- ⇒ Have required calibration weight ready
- ⇒ Press and hold <CAL> key, display, shows "CAL Et"
- ⇒ Release <CAL> key now.
- ⇒ The required calibration weight is shown on the display.
- ⇒ Place calibration weight in center of pan.
- ⇒ The difference between the actual & the measured weight will be displayed.
- ⇒ Press the Tare key when the difference is displayed.
- ⇒ Actual Calibration is perform and Cal done is displayed.

The adjustment can be terminated at any time using the <CANCEL> key. The following message appears : 'Abort'

# Calibration Test Report

If Balance is connected externally to PC or Printer via RS-232/USB Cable, successful or unsuccessful calibration report will be automatically generated after the completion of Calibration process.

## When Standard ON

|                   |            |
|-------------------|------------|
| Calibration :     | External   |
| W-ID              | -----      |
| Temperature       | 32.905°C   |
| Set +             | 200.0000 g |
| Diff. -           | 0.1235 g   |
| External Cal Done |            |
| Diff.             | 0.0000 g   |



## When GLP ON

|                   |            |
|-------------------|------------|
| -----             | -----      |
| 05-Oct-23         | 10:35AM    |
| -----             | ACZET      |
| Model             | CY224C     |
| Ser.No.           | 12345678   |
| Ver.No.           | r.1.1.6.5  |
| Bal. ID.          | S/123      |
| -----             | -----      |
| Product :         | XYZ        |
| Batch ID :        | T123       |
| Sample ID :       | L001       |
| Calibration :     | External   |
| W-ID              | -----      |
| Temperature       | 32.898°C   |
| Set +             | 200.0000 g |
| Diff. -           | 0.1235 g   |
| External Cal Done |            |
| Diff.             | 0.0000 g   |
| -----             | -----      |
| 05-Oct-23         | 10:35AM    |
| Signature :       | -----      |
| -----             | -----      |

## When Customize ON

|                   |               |
|-------------------|---------------|
| -----             | -----         |
| 05-Oct-23         | 10:35AM       |
| -----             | Aczet         |
| -----             | Mumbai, India |
| Model             | CY224C        |
| Ser.No.           | 12345678      |
| Ver.No.           | r.1.1.6.5     |
| Bal. ID.          | S/123         |
| -----             | -----         |
| Product :         | XYZ           |
| Batch ID :        | T123          |
| Sample ID :       | L001          |
| Calibration :     | External      |
| W-ID              | -----         |
| Temperature       | 32.898°C      |
| Set +             | 200.0000 g    |
| Diff. -           | 0.1235 g      |
| External Cal Done |               |
| Diff.             | 0.0000 g      |
| -----             | -----         |
| 05-Oct-23         | 10:35AM       |
| Signature :       | -----         |
| -----             | -----         |

## Key Functionality in User Menu

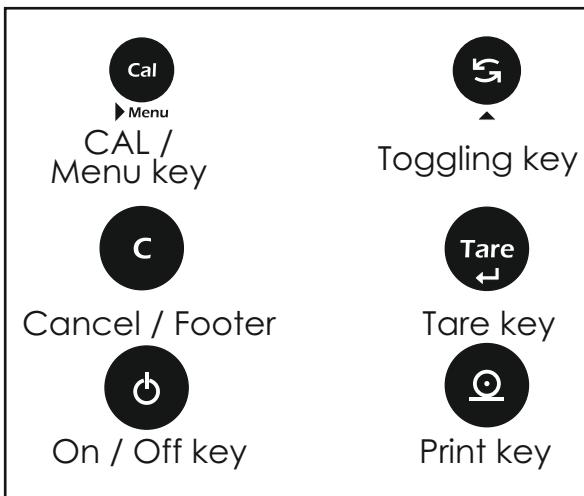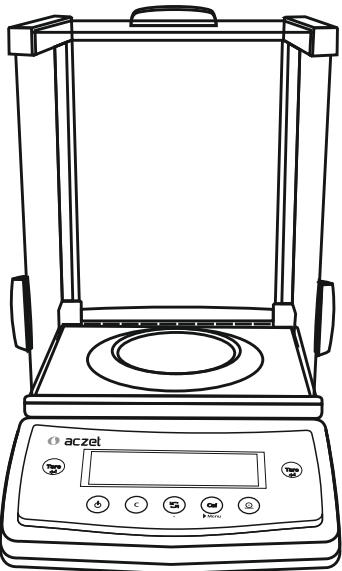


The following section explains key functionality in User Menu mode.


| Menu (called up with   )            |                     |
|-------------------------------------|---------------------|
| Press briefly                       | Press & Hold        |
| On / Off                            |                     |
| Change Sub Menu Setting             |                     |
| Increments the value of digit       |                     |
| Change Main menu options            |                     |
| Shifts the digit from left to right |                     |
| Confirm Setting                     | Store and quit menu |
| Print User Menu                     |                     |
| Quit User Menu                      |                     |

## 5 Overview of Menu

In this menu, you can select unit 1, 2, 3 or Application Program, adjust the stability filter, Calibration choice, Auto Zero Tracking, automatic shutdown and print setting.

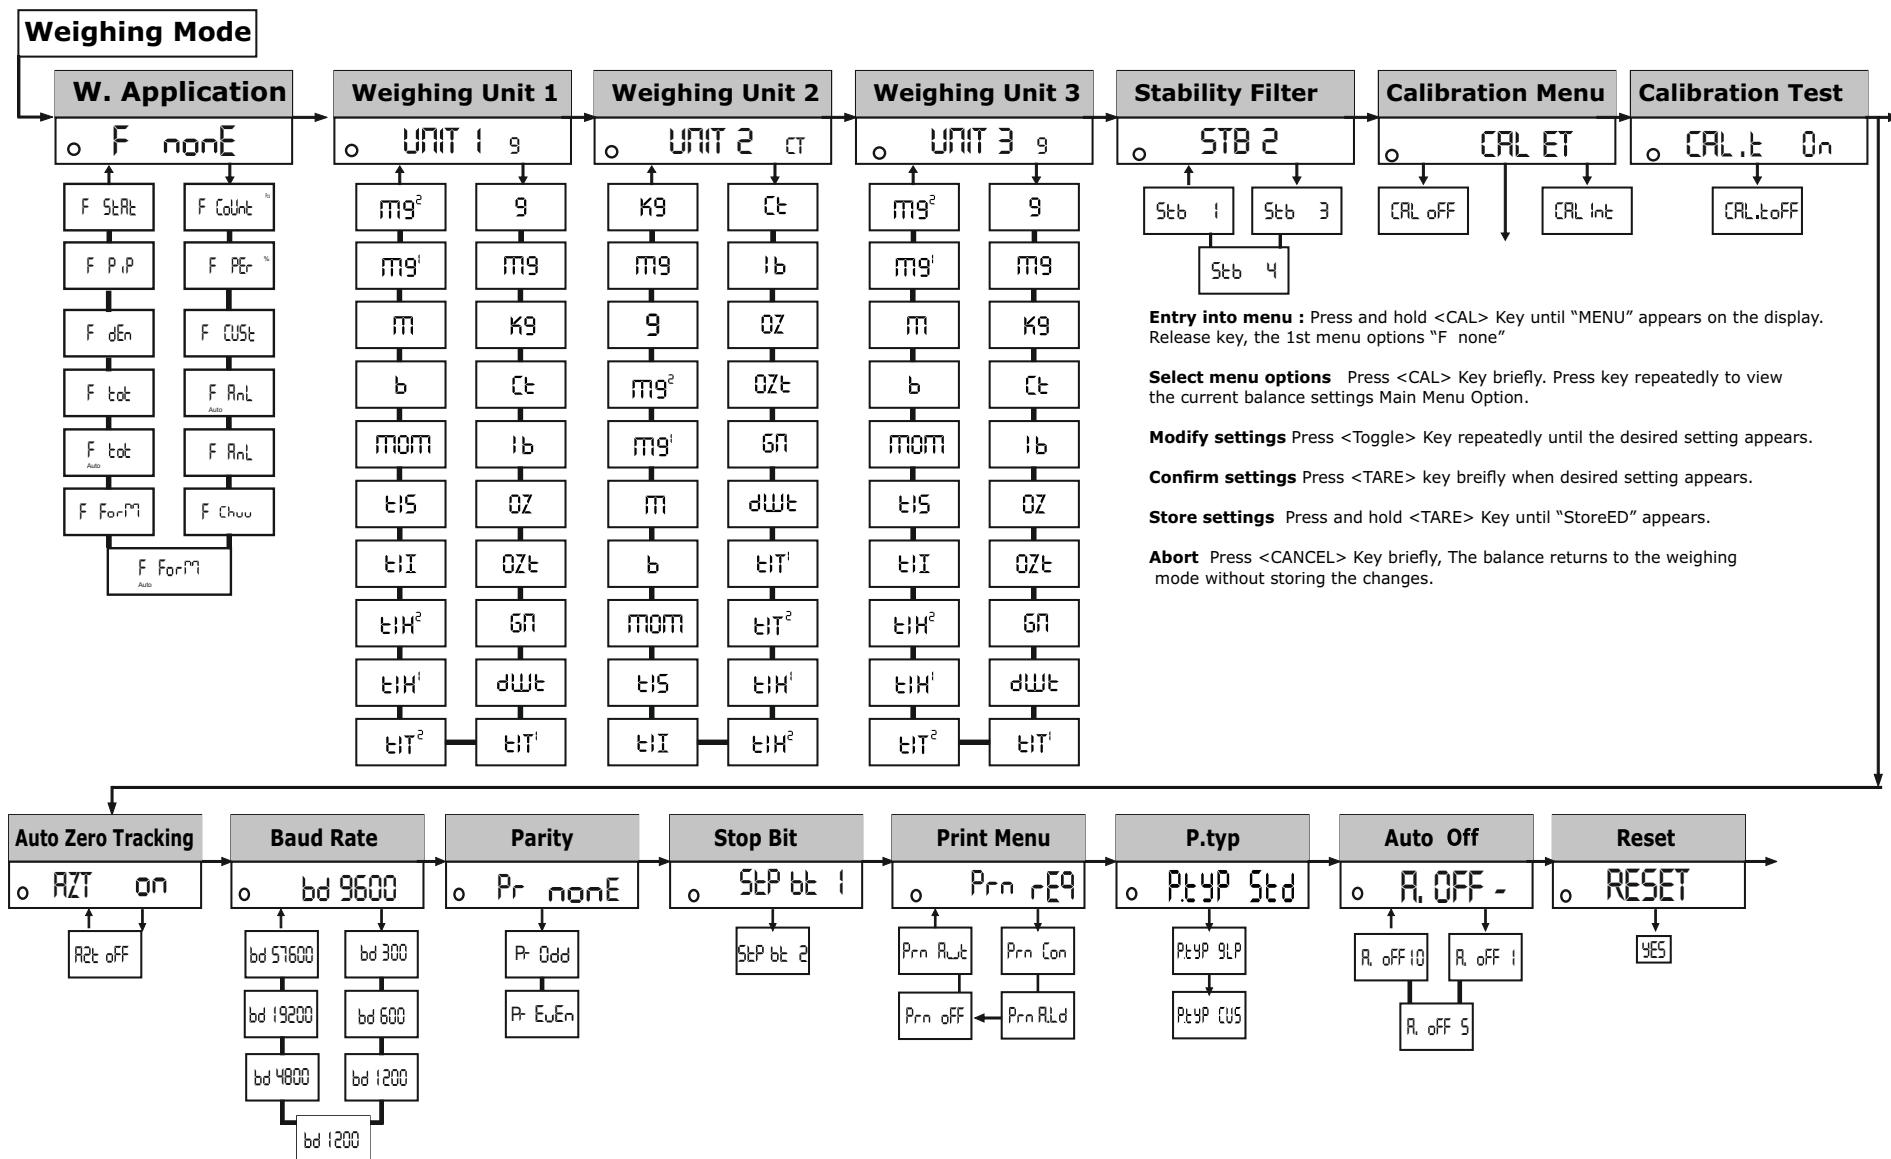

## 5.1 Operating Instruction

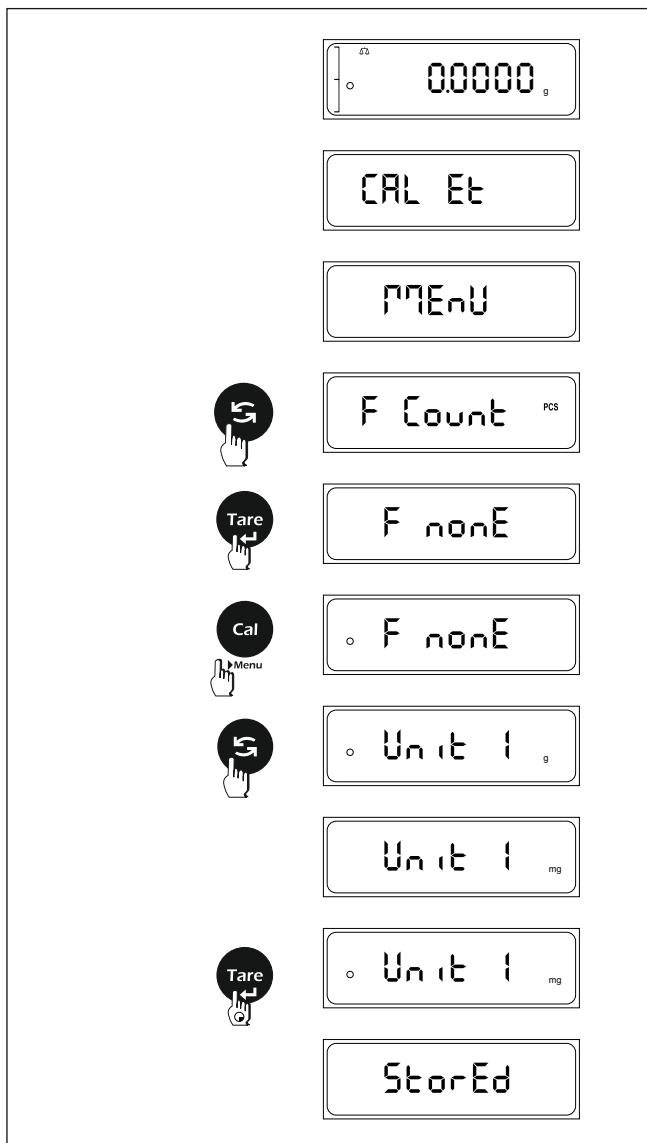


- ⇒ Press & hold CAL Key until "Menu" appears on the display.
- ⇒ Release the CAL Key
- ⇒ Existing preselected function is displayed from among the above mentioned 4 functions. This existing function is displayed with the stability indicator ON
- ⇒ Press Toggle Key to Toggle to the desired functions.
- ⇒ Press Tare Key briefly, once the desired function is displayed. Stability indicator will be ON for that particular function now.
- ⇒ Then Press & hold TARE Key once again till "STORED" is displayed on the display.
  
- ⇒ If more than one changes are to be made within the Menu, make all the desired changes by pressing toggle key to toggle within the SUB-Menus & Pressing Tare key briefly. Stability indicator will be ON for those changed Submenu Options Then finally, pressing & holding TARE key until "Stored" is displayed, will store all the changes made within different menu options.

**Note :** If user did not press & hold <TARE> key & "Stored" message appears on the display then any change made by user will remain unchanged.

Above instructions are to be followed for all menu options except : "Reset"

## 5.2 Description of Menu

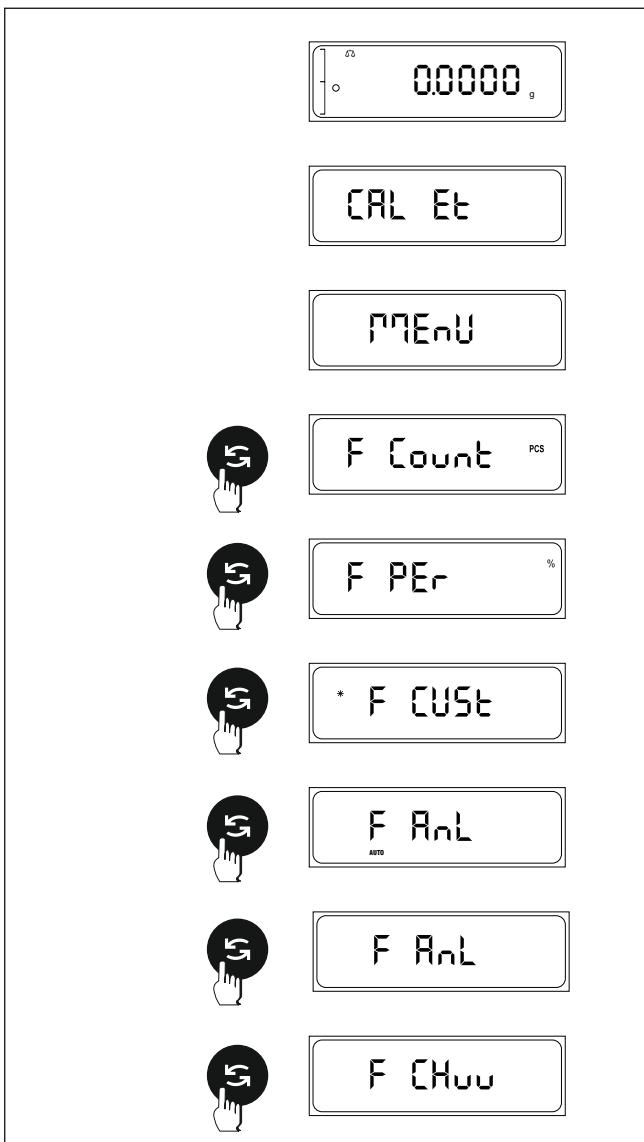

### Application Menu :

#### 5.2.1 Special applications and functions

Your balance can do more than just weighing. Built-in applications and functions expand its possibilities and facilitate your daily work. You will learn these applications and functions in the following Sections.

##### Preselecting a function

In this menu option you can preselect a function which will then be available in the weighing mode (Unit 3) at a keystroke  
The following functions are available.

##### Piece counting

Your balance counts the pieces you add to or remove from the weighing container.


##### Percent weighing

Your balance allows you to weigh in to a preset value or determines percentage weight deviations

**Custom Unit :** Your Balance allows you to weigh in any customized unit.

**Animal Weighing :** Your Balance allows you to weigh animals in motion. You have the option of Auto and Manual Animal Weighing.

**Checkweighing :** Your balance allows you to check whether a sample corresponds to a preset target or is within a specific tolerance range.

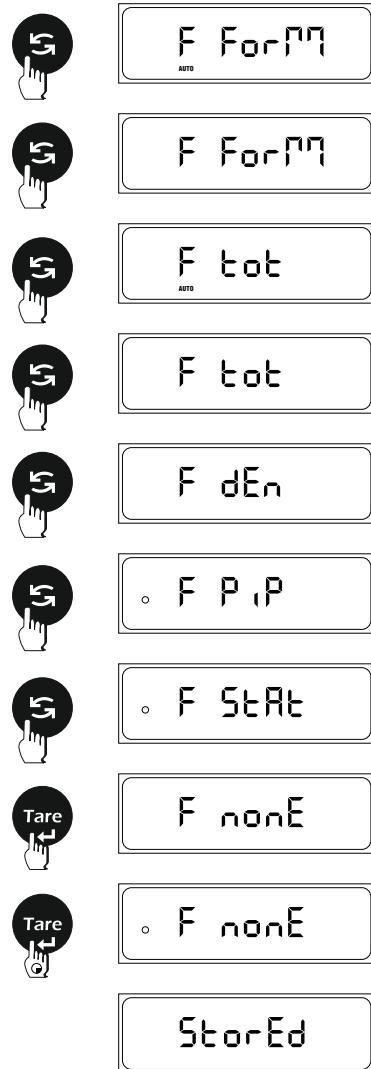

**Formulation :** Your Balance allow individual weighing values to be summed to a total.

**Totalization :** Your balance allows you to weigh, individual weighing in piece which can be summed to a total.

**Density Determination :** Your balance allows you to determine density of solids. Purity of gold can also be determined on the basis of density.

**Pipette Calibration :** Your balance allows you to calibrate the pipette used in laboratories for experimenting with liquids.

**Statistics :** Your balance allows you to obtain the statistics of the weighing data.


#### **No function preselected**

You have no function available in the weighing mode (**factory setting**).

#### **Note :**


Above function will replace preset unit 3 automatically.

### 5.2.2 Unit 1, 2, 3 - selecting

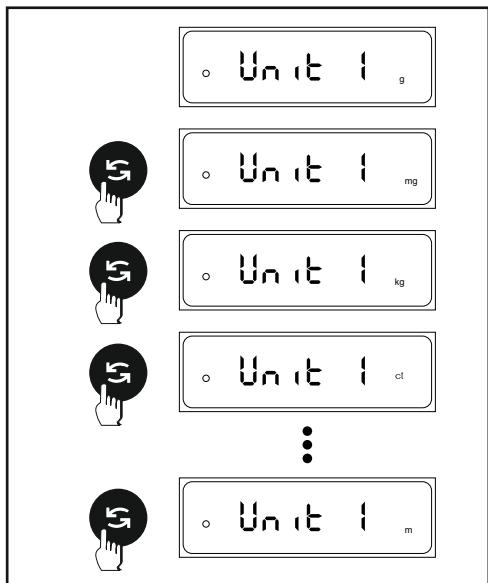

The following weight units can be selected. With **certified balance** the unit selection can be blocked following installation if required by national legislation.


| Unit                             | Conversion factor                  |
|----------------------------------|------------------------------------|
| g gram                           | 1                                  |
| kg kilogram                      | 1 kg = 1000g                       |
| lb pound                         | 1 lb = 453.59237g                  |
| oz ounce                         | 1 oz = 28.349523125g               |
| ozt troy ounce                   | 1 ozt = 31.1034768g                |
| GN grain                         | 1 GN = 0.06479891 g                |
| dwt pennyweight                  | 1 dwt = 1.555173843g               |
| ct carat                         | 1 ct = 0.2g                        |
| mg Milligram                     | 1 mg = 0.001g                      |
| mom momme                        | 1 mom = 3.749999953 g              |
| m mesghal                        | 1 m = 4.6083162                    |
| tIH <sup>1</sup> Hong Kong taels | 1 tIH <sup>1</sup> = 37,42900 g    |
| tIH <sup>2</sup> Hong kong taels | 1 tIH <sup>2</sup> = 37,42900 g    |
| tIS Singapore taels              | 1 tIS = 37.799366256g              |
| tIt <sup>1</sup> Taiwan taels    | 1 tIt <sup>1</sup> = 37.499995313g |
| tIt <sup>2</sup> Taiwan taels    | 1 tIt <sup>2</sup> = 37.499995313g |
| b baht                           | 1 b = 15.1999998438g               |
| mg <sup>1</sup> Myanmar gold     |                                    |
| mg <sup>2</sup> Myanmar gold     |                                    |

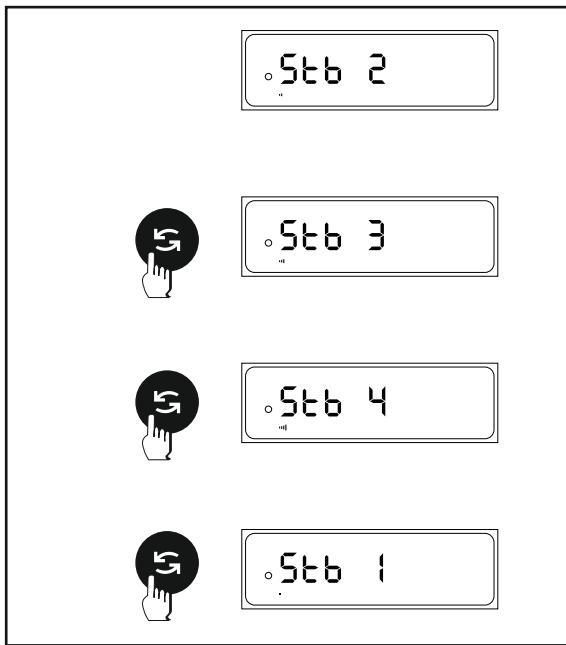

### 5.2.3 Adjusting the stability Filter

You can use the stability Filter to match the balance to the ambient conditions.

- 2 Setting with normal balance surroundings (factory setting)
- 3 Setting with unstable balance surroundings. The balance operates slower but is less sensitive to external influences (vibrations, etc.)
- 4 Setting with extreme unstable balance surroundings. The balance operates even slower but is less sensitive to external influences (vibrations, etc.)
- 1 Setting with very stable balance surroundings. The balance operates very quickly but is sensitive to external influences (vibrations, etc.)

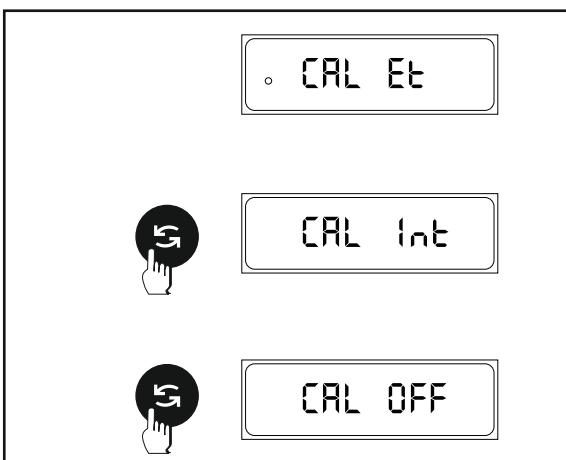

### 5.2.4 Selecting Calibration Option

User can select any of the Two option for Calibration.

**CAL ET** If the user select this option then the machine will perform External Calibration when the CAL key is press & hold to display “CAL Et” & at this moment if user release the key, user can enter into the External calibration.

**CAL OFF** When user press & hold CAL key, directly “Menu” appears on the display without CAL Et option. Thus user cannot enter into the calibration process.

**CAL INT** If the user select this option then the machine will perform **External Calibration** when the CAL key is press & hold to display “CAL Int” & at this moment if user release the key, user can enter into the Internal calibration.



CAL.E OFF



CAL.E On

### 5.2.5 Calibration Test

User Can select any Two calibration test option.

CAL T ON If the user select this option then the machine will perform Calibration Test when the CAL key is press & hold Calibration Test will perform on Internal or External which ever is selected in calibration menu.

CAL T OFF Actual Calibration will be performed When the CAL key is press & hold .



A2t On



A2t OFF

### 5.2.6 Auto Zero Tracking

In this option, user can select whether to enable or disable Auto Zero Tracking (Factory setting is ON)

The auto zero tracking continuously corrects any deviation from the zero point for example which can be caused due to slight contamination (i.e. due to dust particles) on the weighing pan.




## Print Menu

### 5.2.7 Setting baud rate (data transmission rate)

The data transmission rate (baud rate) determines the speed of the transmission via the serial interface.

The unit is baud (1 baud (bd) = 1 bit/second).

The following setting are available. bd 300, bd 600, bd 1200, bd 2400, bd 4800, bd 9600 (default), bd 19200, bd 57600

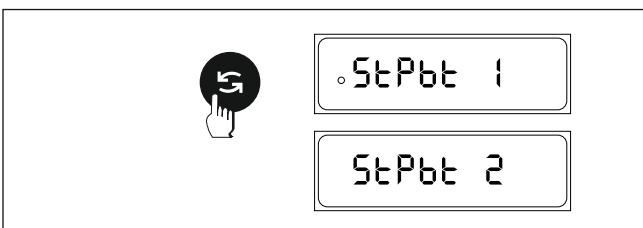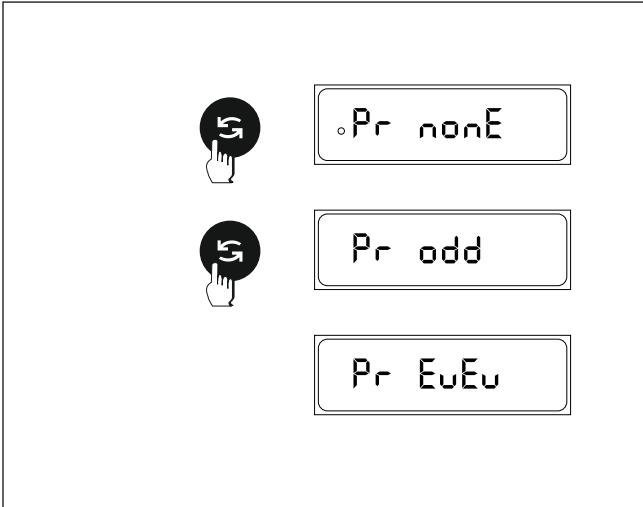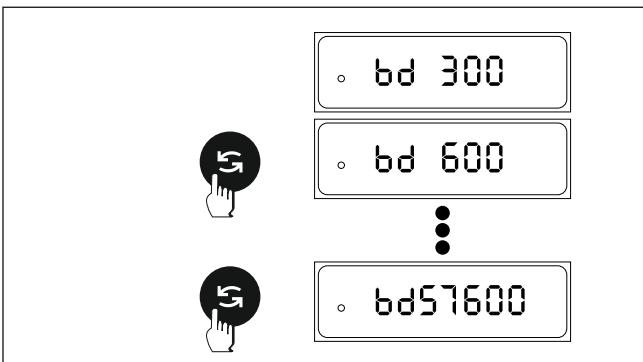

### 5.2.8 Setting Parity

This feature determines the parity of the transmitted data. The following settings are available: Parity, None (default), odd, even.

### 5.2.9 Stop Bit Selection

This setting allows the user to select the stop bit for the transmitted data. The following settings are available: stop bit 1 (Default) and stop bit 2.



Prn req



Prn Con



Prn ALd



Prn Aut

Prn OFF



P.tyP Std



P.tyP GLP

P.tyP CUS

### 5.2.10 Selecting data transfer mode

In this menu block you tell the balance how a value should be transferred to a peripheral device (e.g. computer).

Prn. req The next possible stable value will be transferred after triggering of the Print key.

Prn. Con All Values will be continuously transferred regardless of stability.

Prn. off Data Transfer mode switched off

Prn. Aut Next Possible stable value will be transferred automatically when the display weight changes by + 1d.

Prn. ALd Next possible stable value will be transferred automatically when the display weight changes by +/- 10d

### 5.2.11 Print Type Menu Setting

P.tyP Std If the user select this option then the balance print format are not compliance to ISO/GLP/GMP.

P.tyP GLP If the user select this option then the balance print format are compliance to ISO/GLP/GMP.

P.tyP CUS If the user select this option then the balance print format are compliance to ISO/GLP/GMP.

#### Note

If user selected GLP ON do ensure that user print footer for entering into next transaction and enter into user Menu or Calibration.


### 5.2.12 A. Off - Setting automatic standby

The automatic standby appreciably extends the operating life of your Battery (If Install) (Optional)

The balance will enter stand by mode if A-OFF is activated.

The display on the balance remains zero for a specific time as selected in the A.OFF menu.

- A. Off - : no automatic standby (factory setting)
- A. Off 1 : automatic standby after 1 minutes
- A. Off 5 : automatic standby after 5 minutes
- A. Off 10 : automatic standby after 10 minutes

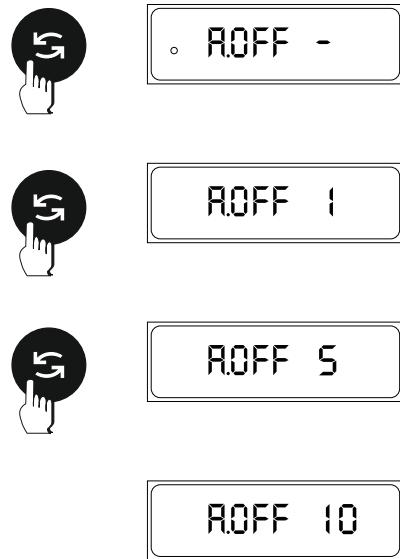


### 5.2.13 Reset of the balance setting

#### Reset balance setting and functions to factory setting (rESEt)

- ⇒ Select “rESEt” and Press <TOGGLE> key breifly, display show “YES”
- ⇒ Press <TARE> key breifly, display show “stored”

The balance is now reset to the factory setting and returns to the weighing mode.\_

#### Factory Setting

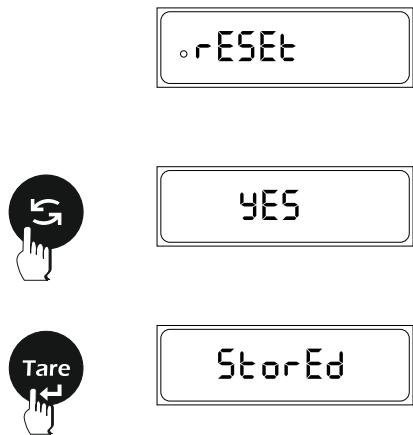

|         |                                   |
|---------|-----------------------------------|
| F none  | No Function                       |
| Unit 1  | gm                                |
| Unit 2  | ct                                |
| Unit 3  | gm                                |
| Stb 2   | balance environment set to Normal |
| CAL Et  | CAL External                      |
| CAL t   | CAL TEST OFF                      |
| Azt ON  | Auto Zero Tracking set ON         |
| bd9600  | Transmission rate                 |
| Pr None | Parity set to none                |
| Stpb1   | Stop bit one                      |
| Print   | Req                               |
| GLP     | OFF                               |
| A. off  | - no automatic standby            |

## USER MENU PRINT OUT

Press the Print Key in the user Menu to Print the current status of user menu.

### When Standard ON

|            |          |
|------------|----------|
| App :      | F Per    |
| Unit1 :    | g        |
| Unit2 :    | ct       |
| Unit3 :    | g        |
| Stb :      | 2        |
| Cal        | Ext      |
| Cal Test : | Off      |
| Azt :      | On       |
| Baudrate : | 9600     |
| Parity :   | None     |
| Stop Bit : | 1        |
| Print :    | Request  |
| P.tyP :    | Standard |
| Auto Off : | Off      |


### When GLP ON

|             |           |
|-------------|-----------|
| -----       | -----     |
| 05-Oct-23   | 10:35AM   |
| -----       | ACZET     |
| -----       | -----     |
| Model       | CY224C    |
| Ser.No.     | 12345678  |
| Ver.No.     | r.1.1.6.5 |
| Bal. ID.    | S/123     |
| -----       | -----     |
| Product :   | XYZ       |
| Batch ID :  | T123      |
| Sample ID : | L001      |
| App :       | F Per     |
| Unit1 :     | g         |
| Unit2 :     | ct        |
| Unit3 :     | g         |
| Stb :       | 2         |
| Cal         | Ext       |
| Cal Test :  | Off       |
| Azt :       | On        |
| Baudrate :  | 9600      |
| Parity :    | None      |
| Stop Bit :  | 1         |
| Print :     | Request   |
| P.tyP :     | GLP       |
| Auto Off :  | Off       |
| -----       | -----     |
| 5-Oct-23    | 10:35AM   |
| Signature : | -----     |
| -----       | -----     |

### When Customize ON

|             |               |
|-------------|---------------|
| -----       | -----         |
| 05-Oct-23   | 10:35AM       |
| -----       | Aczet         |
| -----       | Mumbai, India |
| -----       | -----         |
| Model       | CY224C        |
| Ser.No.     | 12345678      |
| Ver.No.     | r.1.1.6.5     |
| Bal. ID.    | S/123         |
| -----       | -----         |
| Product :   | XYZ           |
| Batch ID :  | T123          |
| Sample ID : | L001          |
| App :       | F Per         |
| Unit1 :     | g             |
| Unit2 :     | ct            |
| Unit3 :     | g             |
| Stb :       | 2             |
| Cal         | Ext           |
| Cal Test :  | Off           |
| Azt :       | On            |
| Baudrate :  | 9600          |
| Parity :    | None          |
| Stop Bit :  | 1             |
| Print :     | Request       |
| P.tyP :     | Customize     |
| Auto Off :  | Off           |
| -----       | -----         |
| 5-Oct-23    | 10:35AM       |
| Signature : | -----         |
| -----       | -----         |

## 6. Functions

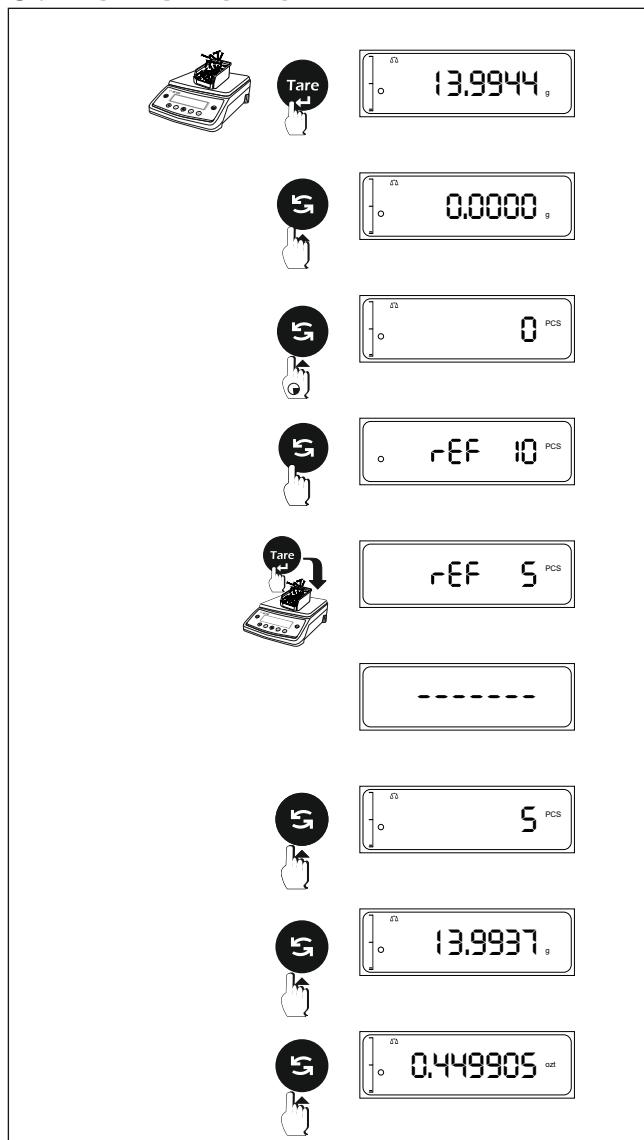

### 6.1 Piece counting

#### Procedure

Piece counting presupposes that you have preselected the “F count” function in the menu


- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “PCS” appears on the display.  
Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.
- ⇒ Your balance suggests the last set reference no. as the reference number.  
You can accept this suggestion or select one of the other reference numbers available (5, 10, 20, 50, 100 pieces, Free, wref, Update) by briefly pressing the <TOGGLE> key.

**Note :** We recommend you to choose a reference number as high as possible as the balance determines the average weight per piece and stores it as the reference weight. As it is seldom, that all pieces weigh exactly the same, the larger the reference number selected, the greater the accuracy of the reference weight. This application assumes uniform weight of each piece.

- ⇒ When you have placed exactly the same number of pieces on the weighing pan as selected reference pieces press TARE key.  
As soon as the weighing result is stable, the calculated average piece weight is accepted as the reference.
- ⇒ After your balance has determined the piece weight, it displays the pieces as per selected number and is now ready for piece counting.  
You can use the <TOGGLE> key at any time to switch the display between the piece number display, weighing unit 1 and weighing unit 2.

**Note :** The current set weight remains stored until it has been redetermined.

### 6.1.1 FREE (Reference settings)

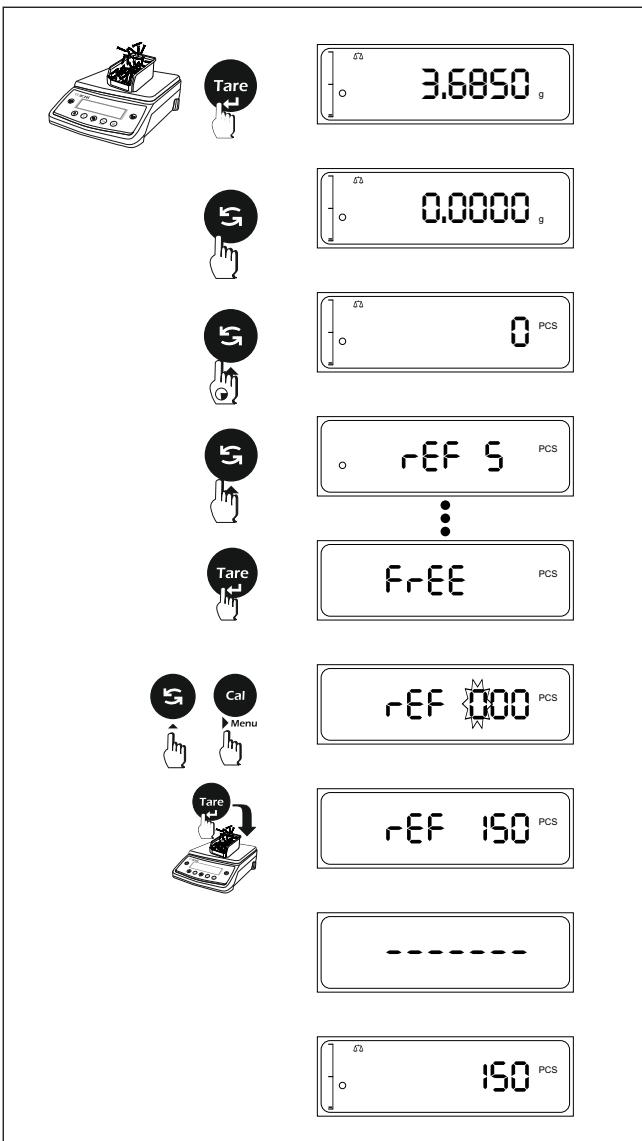

The FREE option allows the user to set any reference other than the fixed available reference.

(Default value is 001 and maximum possible value is 999)


#### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “pcs” appears on the display. Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.
- ⇒ Your balance suggests the last set reference no. as the reference number.
- ⇒ Press the <TOGGLE> key until FREE is displayed.
- ⇒ Press the <TARE> key to enter FREE reference settings.
- ⇒ Last stored FREE value first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press <TOGGLE> key (▲) to change the value of the Flashing digit.
- ⇒ Press <CAL> key (►) to shift the flashing digit from Left to Right
- ⇒ When you have placed exactly the same number of pieces on the weighing pan as set in the FREE setting, press TARE key.

As soon as the weighing result is stable, the calculated average piece weight is accepted as the reference

Now further weighing in PCS will be with respect to the reference calculation based upon the FREE setting.

### 6.1.2 wRef settings

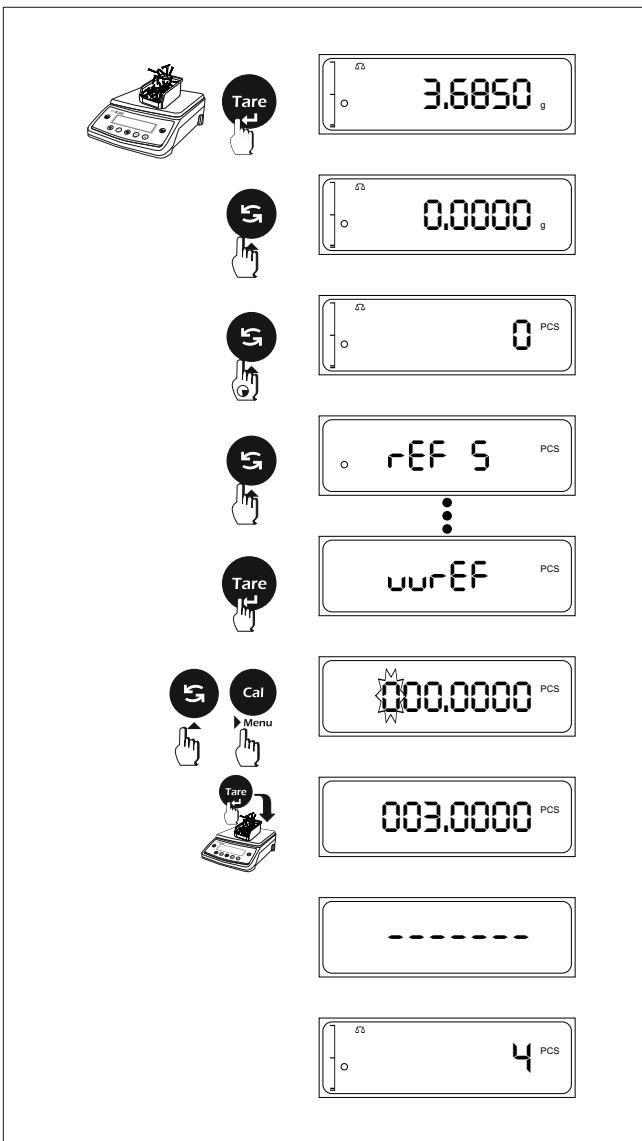


If the piece weight is known, it can be entered directly. To do this, press the TARE key when the system displays **wRef** in the reference menu. An input field appears, in which the piece weight can be entered.

Since the balance does not have to determine a reference by weighing, the result of the piece counting (the number of pieces currently on the weighing pan) is displayed right after the piece weight has been confirmed.

#### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “pcs” appears on the display. Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.
- ⇒ Your balance suggests the last set reference no. as the reference number.
- ⇒ Press the <TOGGLE> key until wRef is displayed.
- ⇒ Press the <TARE> key to enter wRef reference settings.
- ⇒ Last stored wRef value first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press <TOGGLE> key (▲) to change the value of the Flashing digit.
- ⇒ Press <CAL> key (►) to shift the flashing digit from Left to Right
- ⇒ Press the <TARE> key to store the wRef value.

Now further weighing in PCS will be with respect to the wRef value.

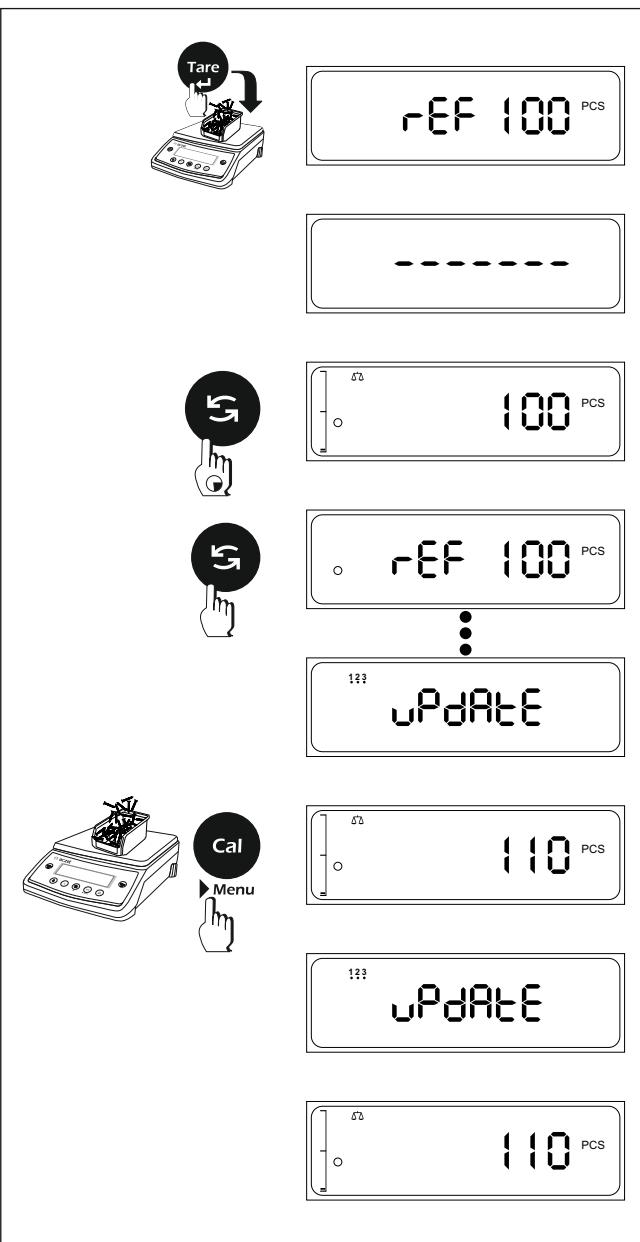

### 6.1.3 Updating Settings

The Update feature improves the precision of piece counting results. The average piece weight (reference) is recalculated with each reference optimization. Because the new pieces that have been placed in the weighing pan increase the basis for the calculation, the references, and therefore the result of the piece count, are more exact.

Select the UPDATE feature from the reference menu. The reference can be updated by pressing the CAL key which is confirmed by the displaying 'UPDATED' on the display.

#### Note

- The number of pieces placed in the weighing pan is larger than the reference piece number shown on the display.
- The number of pieces placed in the weighing pan is not greater than twice the most recently saved reference piece number (e.g. If the display shows 100 pcs the added pieces should not be greater than 200).
- Update feature cannot be selected if the previous selected reference was 'wRef'

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the reference menu of Piece Counting function & make changes in the reference setting, automatically printout is generated on the Peripheral attached.

In the printout, reference number "nRef" and reference weight "wRef" is printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**PCS**), Unit1 and Unit2 and Reference weight is changed

|              |         |
|--------------|---------|
| <i>nRef</i>  | 5 pcs   |
| <i>wRef</i>  | 2.00 g  |
| <i>Qnt +</i> | 5 pcs   |
| <i>Qnt +</i> | 10 pcs  |
| <i>nRef</i>  | 10 pcs  |
| <i>wRef</i>  | 2.00 g  |
| <i>Qnt +</i> | 10 pcs  |
| <i>Qnt +</i> | 5 pcs   |
| <i>nRef</i>  | 50 pcs  |
| <i>wRef</i>  | 0.20 g  |
| <i>Qnt +</i> | 50 pcs  |
| <i>Qnt +</i> | 100 pcs |

### Printout: Counting

nRef + 10 :  
wRef + 21.14 g :  
Qnt + 500 pcs:

Reference sample quantity  
Reference weight  
i.e. weight of one piece  
Calculated quantity

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**PCS**), Unit1 and Unit2 and Reference weight is changed

|                    |           |
|--------------------|-----------|
| -----              | -----     |
| 05-Oct-23          | 10:35AM   |
| -----              | -----     |
| ACZET              |           |
| -----              | -----     |
| <i>Model</i>       | CY224C    |
| <i>Ser.No.</i>     | 12345678  |
| <i>Ver.No.</i>     | r.1.1.6.5 |
| <i>Bal. ID.</i>    | S/123     |
| -----              | -----     |
| <i>Product:</i>    | XYZ       |
| <i>Batch ID:</i>   | T123      |
| <i>Sample ID:</i>  | L001      |
| <i>nRef</i>        | 10 pcs    |
| <i>wRef</i>        | 5.0052 g  |
| <i>Qnt +</i>       | 14 pcs    |
| <i>Qnt +</i>       | 33 pcs    |
| -----              | -----     |
| 05-Oct-23          | 10:35AM   |
| <i>Signature :</i> | -----     |
| -----              | -----     |


### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**PCS**), Unit1 and Unit2 and Reference weight is changed

|                    |           |
|--------------------|-----------|
| -----              | -----     |
| 05-Oct-23          | 10:35AM   |
| -----              | -----     |
| Aczet              |           |
| Mumbai, India      |           |
| -----              | -----     |
| <i>Model</i>       | CY224C    |
| <i>Ser.No.</i>     | 12345678  |
| <i>Ver.No.</i>     | r.1.1.6.5 |
| <i>Bal. ID.</i>    | S/123     |
| -----              | -----     |
| <i>Product:</i>    | XYZ       |
| <i>Batch ID:</i>   | T123      |
| <i>Sample ID:</i>  | L001      |
| <i>nRef</i>        | 5 pcs     |
| <i>wRef</i>        | 3.9979 g  |
| <i>Qnt +</i>       | 5 pcs     |
| <i>Qnt +</i>       | 15 pcs    |
| -----              | -----     |
| 05-Oct-23          | 10:45AM   |
| <i>Signature :</i> | -----     |
| -----              | -----     |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
2) To print footer user will have to Press <CANCEL> key.

## 6.2 Percent Weighing (%)

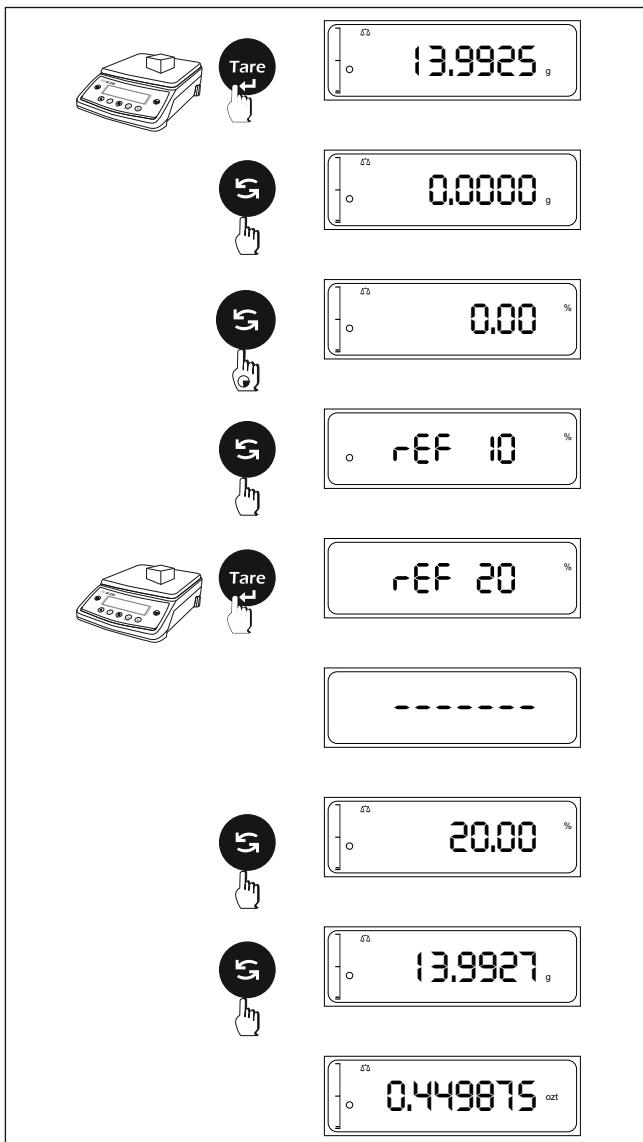

The “Percent weighing” function enables you to weigh in to a preset value (1, 10, 20, 50, 100%, Free, 100r, 100L, AtroM, AtroD) and to determine deviations from this target value.

Percent Weighing (%) presupposes that you have preselected the “F per” function in the menu

### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “PER (%)” appears on the display. Your balance now needs the weight of a reference percent (%).
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference PER (%).
- ⇒ Your balance suggests the last set reference % as the reference percent (%). You can accept this suggestion or select one of the other reference percent (%) available (1, 10, 20, 50, 100 %, Free, 100r, 100L, AtroM, AtroD) by briefly pressing the <TOGGLE> key.
- ⇒ Default is 1%


The FREE option allows the user to set any reference other than the standard available reference. (Default value is 01.00 % and maximum possible value is 99.99%)

- ⇒ Now place reference sample on the pan.
- ⇒ Then press <TARE> key. Until dashes are displayed, your balance is calculating the reference
- ⇒ After your balance has determined the reference weight, it is ready for Percent Weighing.

You can use the <TOGGLE> key at any time to switch the display between the Percent (%) display, weighing unit 1 and weighing unit 2.

**Note :** The current set weight remains stored until it has been redetermined.

### 6.2.1 FREE (Reference settings)

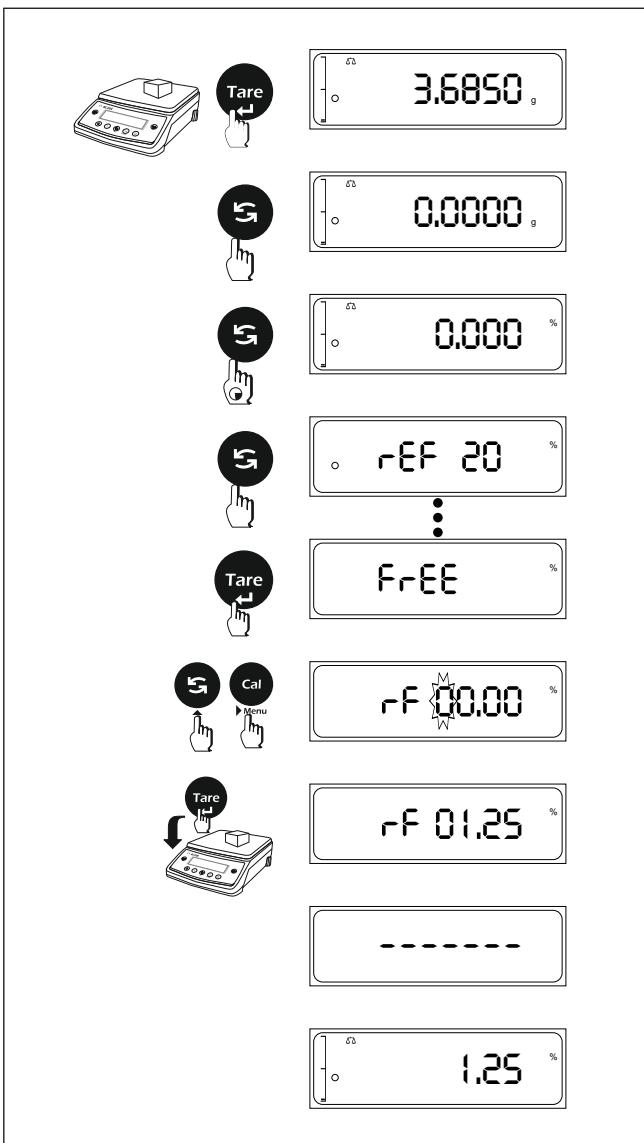

The FREE option allows the user to set any reference other than the standard available reference.

(Default value is 1.00% and maximum possible value is 99.99%)

#### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “**PER**” appears on the display. Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.
- ⇒ Your balance suggests the last set reference no. as the reference number.
- ⇒ Press the <TOGGLE> key until **FREE** is displayed.
- ⇒ Press the <TARE> key to enter FREE reference settings.
- ⇒ Last stored FREE value is displayed. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press <TOGGLE> key (▲) to change the value of the Flashing digit.
- ⇒ Press <CAL> key (►) to shift the flashing digit from Left to Right
- ⇒ When you have placed exactly the same number of pieces on the weighing pan as set in the FREE setting, press TARE key.

As soon as the weighing result is stable, the calculated average piece weight is accepted as the reference

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the reference menu of Percent Weighing function & make changes in the reference setting, automatically printout is generated on the Peripheral attached. in the printout, reference percent "pRef" and reference weight "wRef" is printed. After this user can Press Print key to print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print key to get the print out those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (%), Unit1 and Unit2 and Reference weight is changed

|       |            |
|-------|------------|
| Ref   | 10.00 %    |
| wRef  | 1.00 g     |
| Pct + | 10.00 %    |
| +     | 10.0000 g  |
| +     | 50.0000 ct |
| Pct + | 20.00 %    |
| pRef  | 1.00 %     |
| wRef  | 20.00 g    |
| Pct + | 1.00 %     |
| Pct + | 0.50 %     |

### Printout: Counting

|      |           |   |                       |
|------|-----------|---|-----------------------|
| pRef | 10%       | : | Reference percentage  |
| wRef | + 21.14 g | : | Reference weight      |
| Pct  | + 90.34%  | : | Calculated percentage |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (%), Unit1 and Unit2 and Reference weight is changed

|             |            |
|-------------|------------|
| 05-Oct-23   | 10:35AM    |
| ACZET       |            |
| Model       | CY224C     |
| Ser.No.     | 12345678   |
| Ver.No.     | r.1.1.6.5  |
| Bal. ID.    | S/123      |
| Product :   | XYZ        |
| Batch ID :  | T123       |
| Sample ID : | L001       |
| Ref         | 10.00 %    |
| wRef        | 1.00 g     |
| Pct +       | 10.00 %    |
| +           | 10.0000 g  |
| +           | 50.0000 ct |
| Pct +       | 20.00 %    |
| pRef        | 1.00 %     |
| wRef        | 20.00 g    |
| Pct +       | 1.00 %     |
| Pct +       | 0.50 %     |
| 05-Oct-23   | 10:35AM    |
| Signature : |            |

### When Customize ON


Printouts generated when Unit Toggling is done between Application Unit (%), Unit1 and Unit2 and Reference weight is changed

|               |            |
|---------------|------------|
| 05-Oct-23     | 10:35AM    |
| Aczet         |            |
| Mumbai, India |            |
| Model         | CY224C     |
| Ser.No.       | 12345678   |
| Ver.No.       | r.1.1.6.5  |
| Bal. ID.      | S/123      |
| Product :     | XYZ        |
| Batch ID :    | T123       |
| Sample ID :   | L001       |
| Ref           | 10.00 %    |
| wRef          | 1.00 g     |
| Pct +         | 10.00 %    |
| +             | 10.0000 g  |
| +             | 50.0000 ct |
| Pct +         | 20.00 %    |
| pRef          | 1.00 %     |
| wRef          | 20.00 g    |
| Pct +         | 1.00 %     |
| Pct +         | 0.50 %     |
| 05-Oct-23     | 10:35AM    |
| Signature :   |            |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.

## 6.2.2 Differential Weighing

The Differential Weighing application is used to analyze changes in the weight of one or more samples. The first step is to determine the initial weight of the sample (weighing in). Selected components are then separated from or added to the sample. This includes procedures such as drying, centrifugation, filtering, incineration, vaporization, coating, etc. After the sample has been processed, it is re-weighed (residual weight). The balance then determines the difference between the two weighed values.

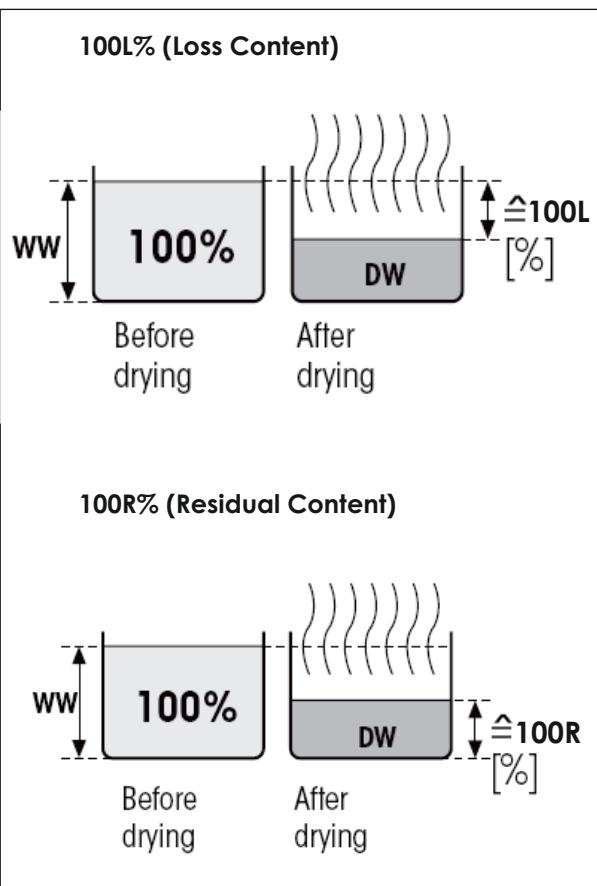

### 100L (Loss)

The moisture content of the sample is displayed (and printed out) as a percentage of the wet weight (= ww = initial weight = 100%). When the results are printed out, the moisture content is designated **100L %" (Loss)** (e.g. -11.35 100.00L%) and shown as a negative value.


$$100L [0...-100\%] = \frac{\text{Dry weight DW} - \text{Wet weight WW}}{\text{Wet weight WW}} * 100\%$$

### 100R (Residue)

The dry content of the sample is displayed (and printed out) as a percentage of the wet weight (= ww = initial weight = 100%). When the results are printed out, the dry content is designated **"100R%" (Residue)** (e.g. 88.65 100.00R%).


$$100R [100...0\%] = \frac{\text{Dry weight DW}}{\text{Wet weight WW}} * 100\%$$

## AtroM Moisture Content

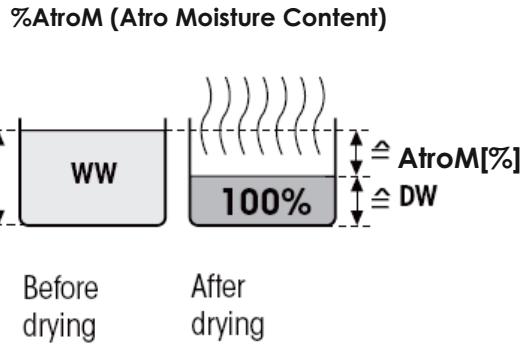

The moisture content of the sample is displayed (and printed out) as a percentage of the dry weight (= DW = final weight = 100%). When the results are printed out, the ATRO moisture content is designated "**AtroM %**" (ATRO Moisture Content) (e.g. -255.33 AtroM %) and shown as a negative value.


$$\text{AtroM [0...-1000%]} = \frac{\text{Dry weight DW} - \text{Wet weight WW}}{\text{Dry weight DW}} * 100\%$$

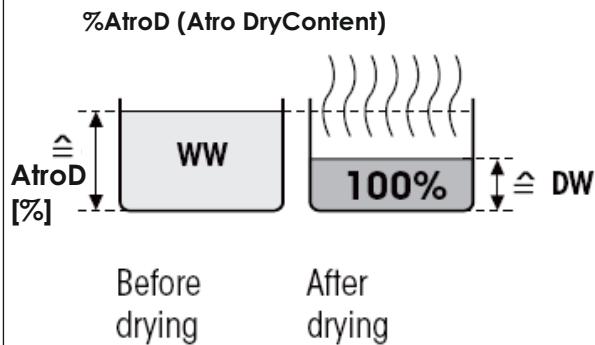

## AtroD Dry Content (Wet weight)

The wet weight of the sample is displayed (and printed out) as a percentage of the dry weight (= DW = final weight = 100%). When the results are printed out, the ATRO dry content is designated "**AtroD %**" (ATRO Dry Content) (e.g. 312.56 AtroD %).

$$\text{AtroD [100...1000%]} = \frac{\text{Wet weight WW}}{\text{Dry weight DW}} * 100\%$$

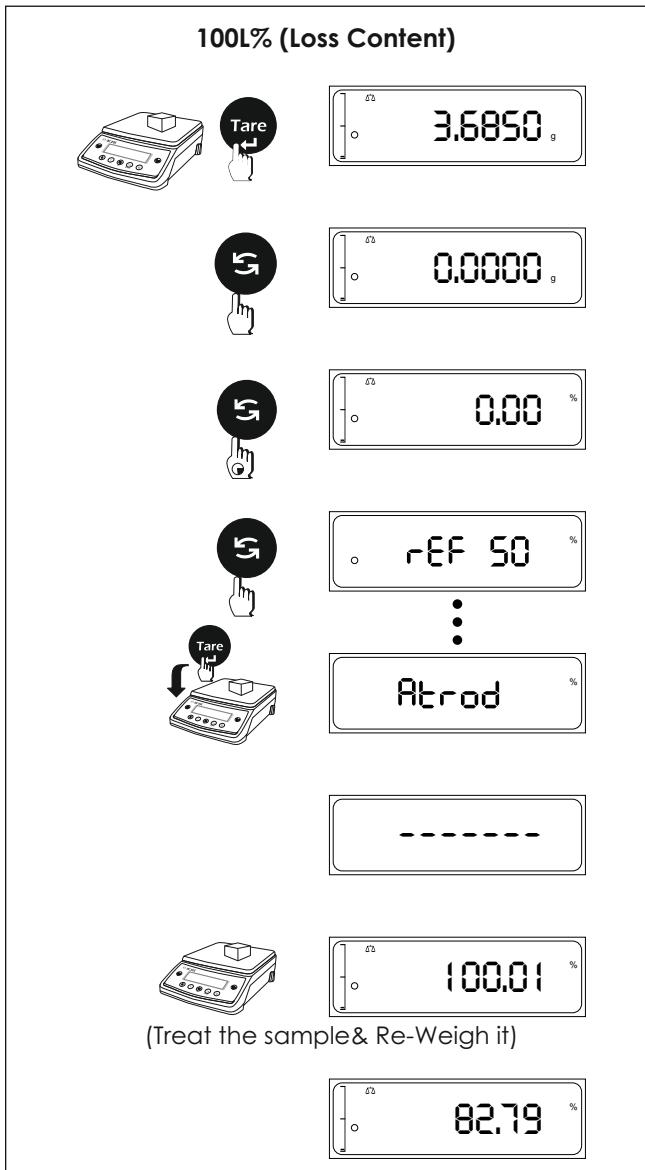

## Percentage Weighing (%) (in 100R / 100L / AtroM / AtroD)

Percent Weighing (%) presupposes that you have preselected the "F per" function in the menu

### Procedure

- ⇒ Press the <TARE> key to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until "PER (%)" appears on the display. Your balance now needs the weight of a reference percent (%).
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference PER (%).
- ⇒ Your balance suggests the last set reference % as the reference percent (%) Press the <TOGGLE> key until the following option is displayed (100R / 100L / AtroM / AtroD)
- ⇒ Now place reference sample on the pan which is to be analyzed (Initial Weight).
- ⇒ Then press <TARE> key. Until horizontal dashes are displayed, your balance is calculating the reference.
- ⇒ After your balance has determined the reference weight, it is ready for Percent Weighing in Differential weighing.
- ⇒ Now treat the sample which includes process like drying, centrifugation, filtering, incineration, vaporization, coating, etc. After the sample has been processed, re-weigh it (residual weight). The balance then determines the difference between the two weighed values.

You can use the <TOGGLE> key at any time to switch the display between the Percent (%) display, weighing unit 1 and weighing unit 2.

**Note:** If the current measured value on display mode is greater or less than the predefined limit value (i.e. greater than 999.99 % or less than -999.99 %) the balance displays Over range (----Or----)

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the reference menu of Percent Weighing function & make changes in the reference setting, automatically printout is generated on the Peripheral attached. In the printout, reference percent "pRef" and reference weight "wRef" is printed. After this user can Press Print Key to Print the reading on the display.

Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Per %**), Unit1 and Unit2 and Reference weight is changed

|       |            |
|-------|------------|
| Ref   | 10.00 %    |
| wRef  | 1.00 g     |
| Pct + | 10.00 g    |
| +     | 10.0000 g  |
| +     | 50.0000 ct |
| Pct + | 20.00 %    |
| pRef  | 1.00 %     |
| wRef  | 20.00 g    |
| Pct + | 1.00 %     |
| Pct + | 0.50 %     |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Per %**), Unit1 and Unit2 and Reference weight is changed

|             |              |
|-------------|--------------|
| 05-Oct-23   | 10:35AM      |
| ACZET       |              |
| Model       | CY224C       |
| Ser.No.     | 12345678     |
| Ver.No.     | r.1.1.6.5    |
| Bal. ID.    | S/123        |
| Product:    | XYZ          |
| Batch ID:   | T123         |
| Sample ID:  | L001         |
| pRef        | 1.00 %       |
| wRef        | 50.0535 g    |
| Pct +       | 1.00 %       |
| +           | 50.0536 g    |
| +           | 1.609260 ozt |
| Pct +       | 1.40 %       |
| Pct +       | 1.40 %       |
| Pct +       | 1.40 %       |
| Pct +       | 3.34 %       |
| 05-Oct-23   | 10:35AM      |
| Signature : |              |


### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Per %**), Unit1 and Unit2 and Reference weight is changed

|                        |           |
|------------------------|-----------|
| 05-Oct-23              | 10:35AM   |
| Aczet<br>Mumbai, India |           |
| Model                  | CY224C    |
| Ser.No.                | 12345678  |
| Ver.No.                | r.1.1.6.5 |
| Bal. ID.               | S/123     |
| Product:               | XYZ       |
| Batch ID:              | T123      |
| Sample ID:             | L001      |
| pRef                   | 10.00 %   |
| wRef                   | 5.0054 g  |
| Pct +                  | 1.00 %    |
| +                      | 50.0536 g |
| Pct +                  | 1.40 %    |
| 05-Oct-23              | 10:45AM   |
| Signature :            |           |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
2) To print footer user will have to Press <CANCEL> key.

## 6.3 Custom Unit

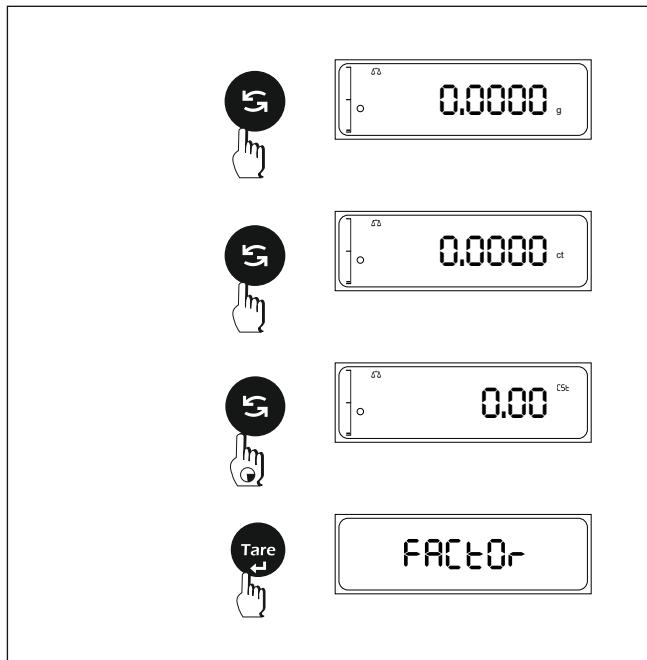


The custom unit feature enables you to perform weighing in a customized unit i.e. weighing can now be performed in a unit other than standard available 15 units.

### Procedure

Custom unit presupposes that you have selected the 'F Cust' in the user menu.

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until "CSt" appears on the display.  
Your balance now needs conversion factor, accuracy and LSD to perform weighing in custom unit.
- ⇒ Press and hold the <TOGGLE> key to browse through the custom unit setting menu.  
Your balance suggests the last stored values for the factor, accuracy and LSD.
- ⇒ Press the <TARE> key to enter the specific setting.

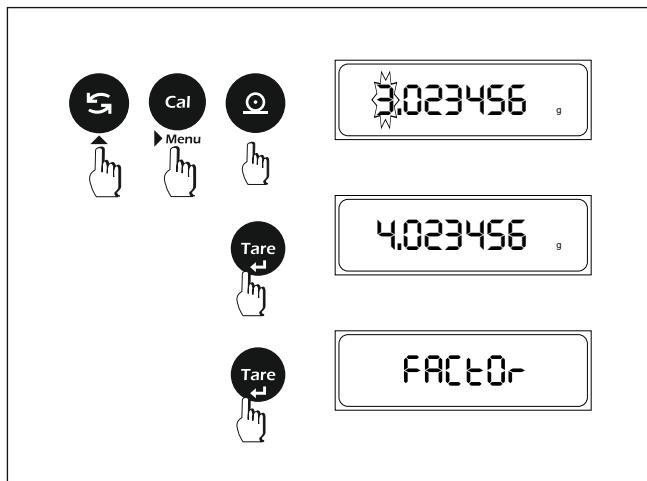


### Factor Setting

The factor value can be set to any user defined value except for zero.

- ⇒ Press the <TARE> key to enter the factor setting.
- ⇒ Press the <TOGGLE> key (▲) to change the value of the flashing digit.
- ⇒ Press the <CAL> key (►) to change the flashing digit from left to right.
- ⇒ Press the <PRINT> key to shift the decimal position in a cyclic way.
- ⇒ After proper setting of factor press the <TARE> key.

**Note:** Please refer error conditions for errors occurred in storing the Factor, Accuracy and LSD settings.

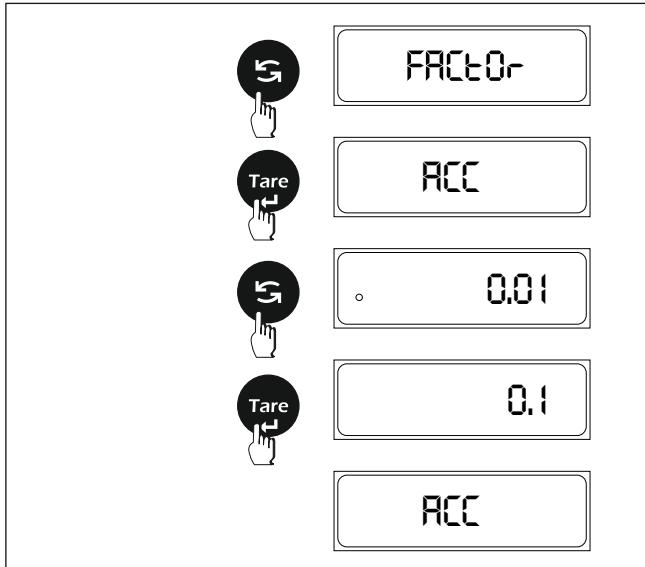

## Accuracy Setting

- ⇒ Press the <TARE> key when the Acc is displayed.
- ⇒ Press the <TOGGLE> key to browse through the standard available accuracy.
- ⇒ You can select any of the standard accuracy with the help of <TARE> key.

Standard accuracies available are

**0.000001, 0.00001, 0.0001, 0.001, 0.01, 0.1, 1, 10, 100, 1000**

The stability indicator alongside indicates the selected accuracy.

The Accuracy Setting is for display purposes and not for calculation of Custom unit.

## LSD Setting

- ⇒ Press the <TARE> key when LSD is displayed.
- ⇒ Press the <TOGGLE> key to browse through the standard available LSD's.
- ⇒ You can select any of the standard available LSD (Least significant Digit) with the help of <TARE> key.

Standard LSD's available are

**1, 2, 5, 10, 20, 50, 100**

The stability indicator alongside indicates the selected LSD.

To store the Factor, Accuracy and LSD values, press and hold the <TARE> key when the display shows Factor or Acc or LSD

The default settings are

**Factor = 1.0000 (i.e. 1 gram)**

**Accuracy = 0.01**

**LSD = 1**

E.g. If the settings are as follows,

Factor = 1.02356

Accuracy = 0.00

LSD = 50

Now if 50 gm of weight is loaded on the pan the calculation for displayed weight will be as follows,

Weight \* Factor

= 50 \* 1.023456

= 51.1728

The displayed weight will be 51.150

The second digit after decimal point will change in multiples of 5 because,

Accuracy \* LSD

= 50 \* 0.001

= 0.05

You can use the <TOGGLE> key at any time to switch the display between custom unit display, weighing unit 1 and weighing unit 2. User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by Cancel key and balance shows Current weights.

If the balance is connected eternally to PC or Printer through RS-232/USB then, whenever user enter into the Custom Unit Menu & make changes in the Factor, Accuracy and LSD setting, automatically printout is generated on the Peripheral attached.

In the printout, the new Factor, Accuracy and LSD values are printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Cst**), Unit1 and Unit2

|          |            |
|----------|------------|
| Factor   | 3.023456   |
| Accuracy | 0.1        |
| Lsd      | 2          |
| +        | 151.2 cst  |
| +        | 50.0000 g  |
| +        | 250.000 ct |
| Factor   | 1.023456   |
| Accuracy | 0.001      |
| Lsd      | 50         |
| +        | 61.400 cst |
| +        | 51.200 cst |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Cst**), Unit1 and Unit2

|             |            |
|-------------|------------|
| -----       | -----      |
| 05-Oct-23   | 10:35AM    |
| -----       | -----      |
| ACZET       |            |
| -----       | -----      |
| Model       | CY224C     |
| Ser.No.     | 12345678   |
| Ver.No.     | r.1.1.6.5  |
| Bal. ID.    | S/123      |
| -----       | -----      |
| Product:    | XYZ        |
| Batch ID :  | T123       |
| Sample ID : | L001       |
| Factor      | 3.023456   |
| Accuracy    | 0.01       |
| Lsd         | 5          |
| +           | 293.60 cst |
| +           | 445.05 cst |
| +           | 147.2106 g |
| -----       | -----      |
| 05-Oct-23   | 10:35AM    |
| -----       | -----      |
| Signature : |            |
| -----       | -----      |

### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Cst**), Unit1 and Unit2

|               |            |
|---------------|------------|
| -----         | -----      |
| 05-Oct-23     | 10:35AM    |
| -----         | -----      |
| Aczet         |            |
| Mumbai, India |            |
| -----         | -----      |
| Model         | CY224C     |
| Ser.No.       | 12345678   |
| Ver.No.       | r.1.1.6.5  |
| Bal. ID.      | S/123      |
| -----         | -----      |
| Product:      | XYZ        |
| Batch ID :    | T123       |
| Sample ID :   | L001       |
| Factor        | 3.023456   |
| Accuracy      | 0.1        |
| Lsd           | 2          |
| +             | 293.6 cst  |
| +             | 147.2106 g |
| -----         | -----      |
| 05-Oct-23     | 10:45AM    |
| -----         | -----      |
| Signature :   |            |
| -----         | -----      |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.

## 6.4 Animal Weighing

The animal weighing feature enables you to perform weighing of unstable samples (live animals). The balance calculates the weight as the average of a defined number of individual weighing operations.

You can select from the two available animal weighing modes i.e. Auto animal weighing and manual weighing.

The weighing unit for animal weighing will be the same as selected for unit 1.


For Animal Weighing Process to start two conditions should be satisfied, the weight of the animal kept on the pan should be higher than 100 display increment i.e. if the balance capacity is 300 gm and accuracy is 0.0001 gm, then in Animal weighing process the weight of the animal should be above  $100 * 0.0001 = 0.001$  g and when two successive weight measured are within predefined tolerance range.

Number of weighing operations for calculation of an average **Cnt** be set before the beginning of each series.

Balance returns to the basic weighing mode when unloaded; i.e., when the load is below the unload threshold.

The Unload threshold is 50 display intervals.

#### 6.4.1 Manual Animal Weighing

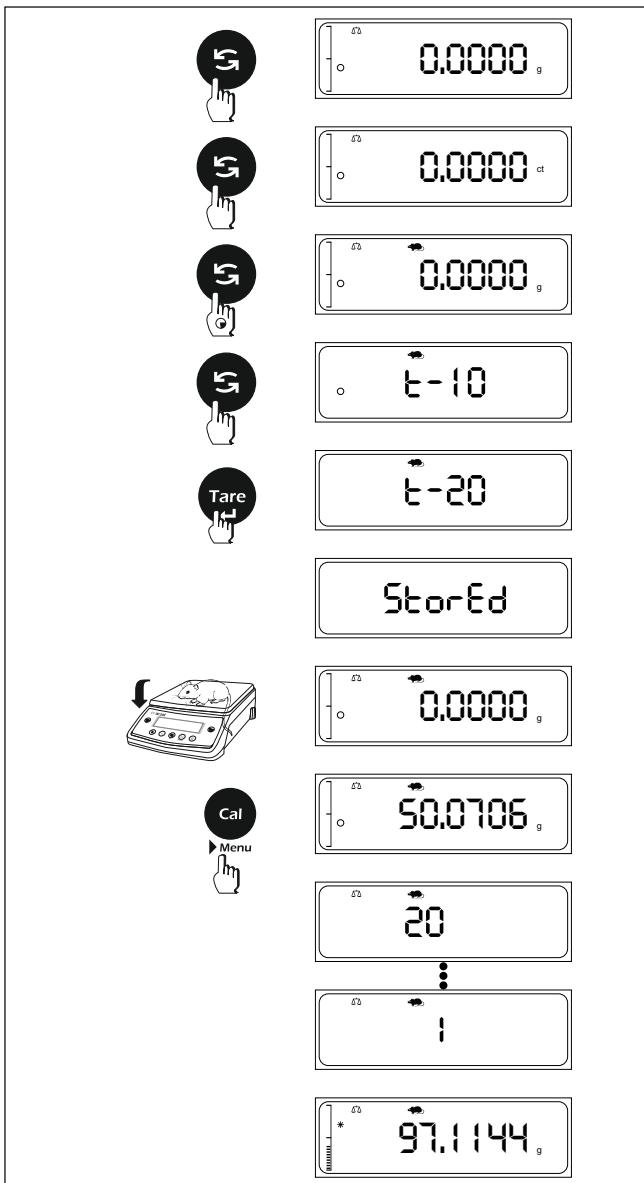

Manual Animal Weighing presupposes that you have selected the 'F Anl' in the user menu.

##### Procedure


- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until " symbol appears on the display. Your balance now needs to set the countdown value.
- ⇒ Press and hold the <TOGGLE> key to enter countdown options. The entire menu can be accessed by pressing the <TOGGLE> key. The stability symbol indicates the currently selected countdown value.
- ⇒ Press the <TARE> key to select specific countdown value.
- ⇒ Keep the animal on the pan, press the <CAL> key to start the animal weighing process when both the condition required for animal weighing are met the countdown process will start, when the countdown time ends the average weight on animal is displayed with the display locked with flashing animal symbol.

Locked display is indicated by the flashing animal and AUTO symbol.

The countdown options available are,

- t-5
- t-10 (Default)
- t-20
- t-50
- t-100

You can use the <TOGGLE> key at any time to switch the display between animal weighing, weighing unit 1 and weighing unit 2. User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by Cancel key and balance shows Current weights.

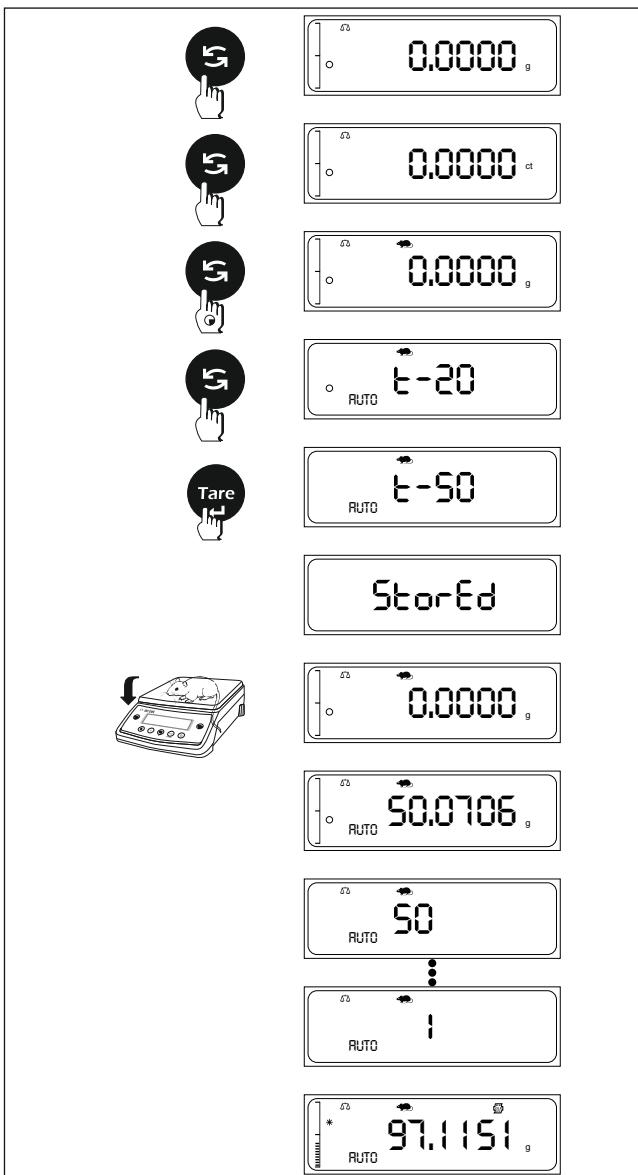

#### 6.4.2 Auto Animal Weighing

Auto Animal Weighing presupposes that you have selected the 'F Anl AUTO' in the user menu. Auto animal weighing proves to be beneficial when the balance is used majority for animal weighing and less for simple weighing thus reducing the time required for animal weighing.

##### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “ ” and “**AUTO**” symbol appears on the display.

Your balance now needs to set the countdown value.

- ⇒ Press and hold the <TOGGLE> key to enter countdown menu. The entire menu can be accessed by the <TOGGLE> key.
- The stability symbol indicates the currently selected countdown value.
- ⇒ Press the <TARE> key to select specific countdown value.
- ⇒ Keep the animal on the pan, when both the condition required for animal weighing are met the countdown process will start, when the countdown time ends the average weight on animal is displayed with the display locked.

Thus there is no need of pressing a key to start the countdown process in the auto animal weighing mode.

Locked display is indicated by the flashing animal and AUTO symbol.

The countdown options available are,

##### **t-5 (Auto), t-10 (Auto) Default, t-20 (Auto), t-50 (Auto), t-100(Auto)**

You can use the <TOGGLE> key at any time to switch the display between animal weighing, weighing unit 1 and weighing unit 2. User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by Cancel key and balance shows Current weights.

If the balance is connected eternally to PC or Printer through RS-232/USB then, whenever user enter into the Countdown Menu of Animal Weighing & make changes in the countdown time automatically printout is generated on the Peripheral attached.

In the printout, the new countdown value '**mDef**' is printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Anl**), Unit1 and Unit2 and Reference Weight is changed

|       |              |
|-------|--------------|
| Cnt   | 20           |
| xNt + | 50.0709 g    |
| +     | 50.0715 g    |
| +     | 250.357z5 ct |
| xNt + | 50.0709 g    |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Anl**), Unit1 and Unit2 and Reference Weight is changed

|                   |              |
|-------------------|--------------|
| -----             | -----        |
| 05-Oct-23         | 10:35AM      |
| ACZET             |              |
| Model             | CY224C       |
| Ser.No.           | 12345678     |
| Ver.No.           | r.1.1.6.5    |
| Bal. ID.          | S/123        |
| -----             | -----        |
| Product:          | XYZ          |
| Batch ID :        | T123         |
| Sample ID :       | L001         |
| Cnt               | 10           |
| xNt +             | 97.1141 g    |
| +                 | 97.1141 g    |
| +                 | 3.122290 ozt |
| xNt +             | 97.1141 g    |
| -----             | -----        |
| 05-Oct-23         | 10:35AM      |
| Signature : ----- |              |
| -----             | -----        |

### Printout: Counting

|       |           |   |                                  |
|-------|-----------|---|----------------------------------|
| Cnt   | 20        | : | Number of subweighing operations |
| xNt + | 50.0709 g | : | Calculated Average               |

### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Anl**), Unit1 and Unit2 and Reference Weight is changed

|                        |           |
|------------------------|-----------|
| -----                  | -----     |
| 05-Oct-23              | 10:35AM   |
| Aczet<br>Mumbai, India |           |
| Model                  | CY224C    |
| Ser.No.                | 12345678  |
| Ver.No.                | r.1.1.6.5 |
| Bal. ID.               | S/123     |
| -----                  | -----     |
| Product:               | XYZ       |
| Batch ID :             | T123      |
| Sample ID :            | L001      |
| Cnt                    | 10        |
| xNt +                  | 50.0517 g |
| -----                  | -----     |
| 05-Oct-23              | 10:45AM   |
| Signature : -----      |           |
| -----                  | -----     |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
2) To print footer user will have to Press <CANCEL> key.

## 6.5 Formulation

The formulation feature allows individual weighing values to be summed to a total.

User can select from two available formulation modes i.e. Manual formulation and auto formulation.

Maximum no of weights that can be summed is 99.


Store component weights with

- Display zeroed automatically after value is stored, and
- Automatic printout (print application parameters)
- Of the last component weight (net value) and
- Of the total weight (tare value)

Clear component memory when weighing series is canceled by pressing CANCEL key

**Note :**

- Individual weights can be added into summation only if the weights are greater than 20d, this is indicated by '↓' symbol.
- The weighing unit for formulation will be the same as selected.

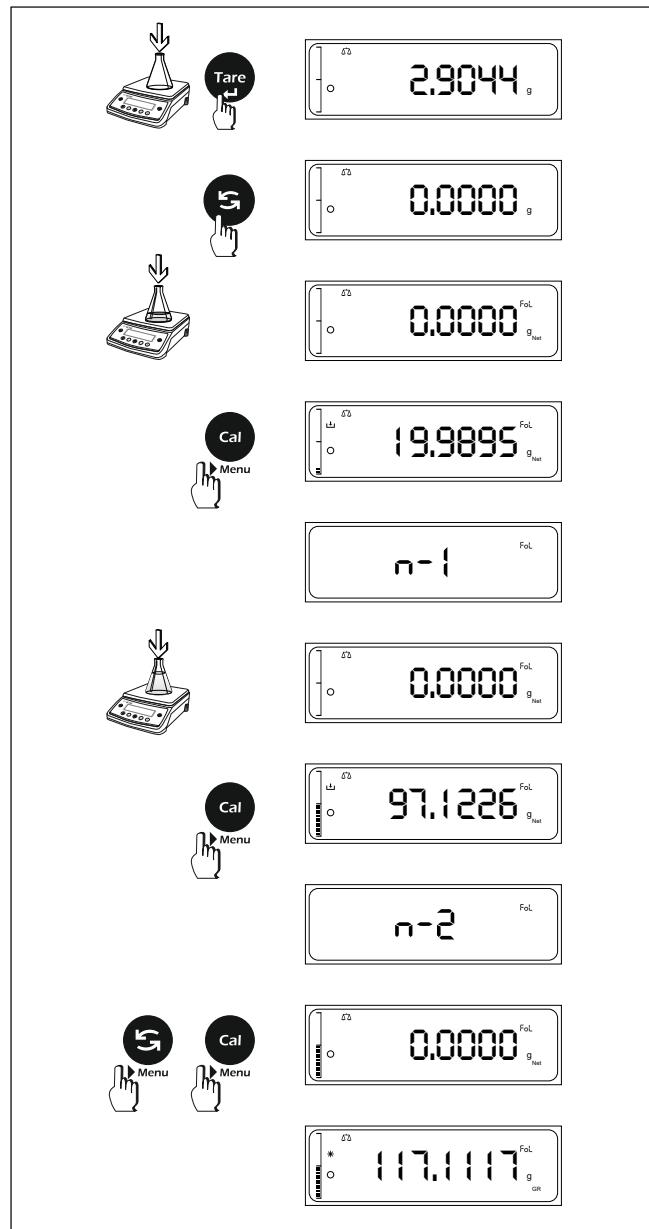

### 6.5.1 Manual Formulation

Manual formulation presupposes that you have selected the 'F Form' in the user menu.

#### Procedure

Place the empty container on the pan.

- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until Fol is displayed on the display.
- ⇒ Add weight on the pan. Weight can be added to summation when '↓' is displayed on the display i.e. when it is greater than 20d.
- ⇒ Press the <CAL> key to store the weight, the balance displays "n-1" indicating that 1st weight is stored. The weight is tarred automatically and simultaneously print command is given.

E.g. if 9.9968 gm is added the printer output is as follows


|     |   |           |
|-----|---|-----------|
| N1  | : | 9.9968 g  |
| Tot | : | +9.9968 g |

Further addition of weights will give the following output (addition of 20.0070 gm).

|     |   |            |
|-----|---|------------|
| N2  | : | 20.0070 g  |
| Tot | : | +39.0038 g |

- ⇒ To view the total weight, press the <CAL> and <TOGGLE> key together. The print command is given automatically

|     |   |             |
|-----|---|-------------|
| N   | 2 |             |
| Tot | : | + 39.0038 g |

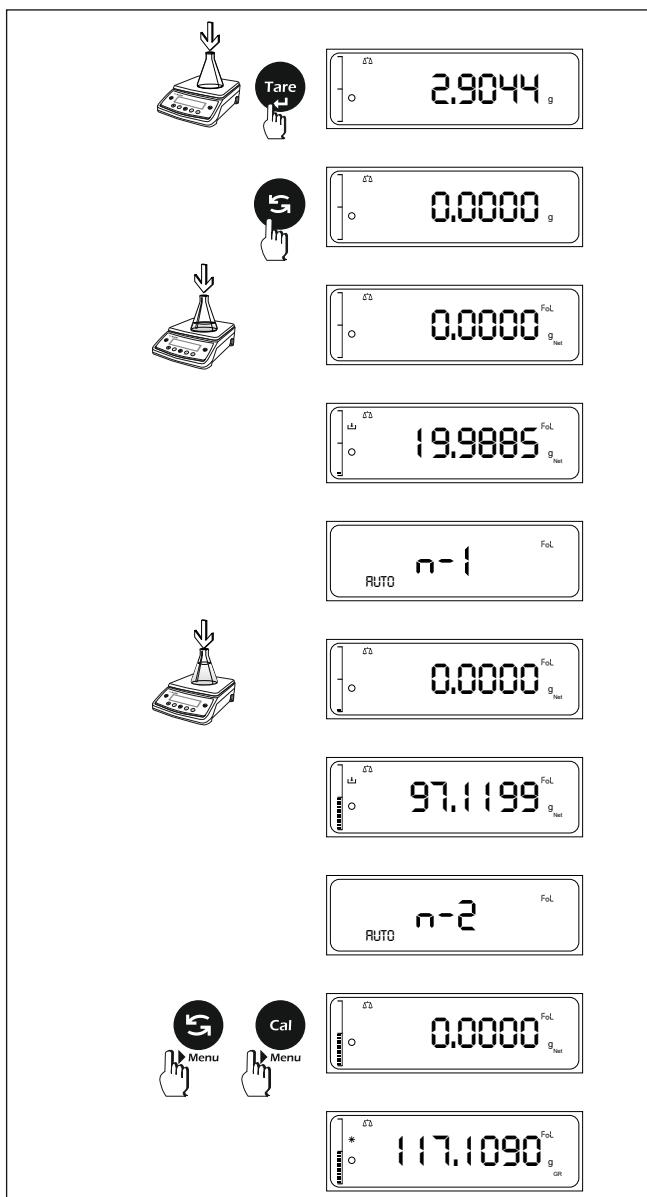

### 6.5.2 Auto Formulation

Auto formulation presupposes that you have selected the 'F Form AUTO' in the user menu.

Auto formulation proves to be beneficial when the balance is used in majority for formulation weighing and less for simple weighing thus reducing the time required for formulation as compared to manual formulation.

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until Fol and AUTO is displayed on the display.
- ⇒ Add weight on the pan. Weight can be added to summation when “” is displayed on the display i.e. when it is greater than 20d.
- ⇒ When the weight is stable the weight is stored in the formulation procedure and the balance displays “n-1” indicating that 1st weight is stored. The weight is tarred automatically and simultaneously print command is given. Thus there is no need to press any to start the auto formulation procedure.

You can use the <TOGGLE> key at any time to switch the display between formulation, weighing unit 1 and weighing unit 2. User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by CANCEL key and balance shows Current weights.

If the balance is connected eternally to PC or Printer through RS-232/USB then, whenever user adds weight to the formulation procedure automatically printout is generated on the Peripheral attached.

In the printout, the component added '**N x**' along with the total sum '**Tot**' is printed. After this user can Press Print Key to Print the reading on the display.

Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**For1**), Unit1 and Unit2 and Reference Weight is changed

|              |             |
|--------------|-------------|
| <i>N1 +</i>  | 20.0000 g   |
| <i>Tot +</i> | 20.0000 g   |
| <i>+</i>     | 20.0000 g   |
| <i>+</i>     | 100.0000 ct |
| <i>N2 +</i>  | 50.0000 g   |
| <i>Tot +</i> | 70.0000 g   |
| <i>N</i>     | 2           |
| <i>Tot +</i> | 70.0000 g   |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**For1**), Unit1 and Unit2 and Reference Weight is changed

|              |            |
|--------------|------------|
| -----        | -----      |
| 05-Oct-23    | 10:35AM    |
| -----        | ACZET      |
| Model        | CY224C     |
| Ser.No.      | 12345678   |
| Ver.No.      | r.1.1.6.5  |
| Bal. ID.     | S/123      |
| -----        | -----      |
| Product:     | XYZ        |
| Batch ID :   | T123       |
| Sample ID :  | L001       |
| <i>N1 +</i>  | 97.1133 g  |
| <i>Tot +</i> | 97.1133 g  |
| <i>N2 +</i>  | 50.0944 g  |
| <i>Tot +</i> | 147.2077 g |
| <i>N3 +</i>  | 20.0160 g  |
| <i>Tot +</i> | 167.2237 g |
| <i>N</i>     | 3          |
| <i>Tot +</i> | 167.2237 g |
| -----        | -----      |
| 05-Oct-23    | 10:35AM    |
| -----        | -----      |
| Signature :  | -----      |
| -----        | -----      |

### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**For1**), Unit1 and Unit2 and Reference Weight is changed


|              |               |
|--------------|---------------|
| -----        | -----         |
| 05-Oct-23    | 10:35AM       |
| -----        | Aczet         |
| -----        | Mumbai, India |
| Model        | CY224C        |
| Ser.No.      | 12345678      |
| Ver.No.      | r.1.1.6.5     |
| Bal. ID.     | S/123         |
| -----        | -----         |
| Product:     | XYZ           |
| Batch ID :   | T123          |
| Sample ID :  | L001          |
| <i>N1 +</i>  | 97.1133 g     |
| <i>Tot +</i> | 97.1133 g     |
| <i>N2 +</i>  | 50.0945 g     |
| <i>Tot +</i> | 147.2078 g    |
| <i>N3 +</i>  | 20.0161 g     |
| <i>Tot +</i> | 167.2239 g    |
| <i>N</i>     | 3             |
| <i>Tot +</i> | 167.2239 g    |
| -----        | -----         |
| 05-Oct-23    | 10:45AM       |
| -----        | -----         |
| Signature :  | -----         |
| -----        | -----         |

### Printout Configuration

|                 |                              |
|-----------------|------------------------------|
| N1 + 20.0000 g  | 1st component and its weight |
| Tot + 20.0000 g | Sum of components            |
| N2 + 50.0000 g  | 2nd component and its weight |
| Tot + 70.0000 g | Sum of components            |
| N 2             | Total number of components   |
| Tot + 70.0000 g | Total formulation weight     |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press **<CANCEL>** key.

## 6.6 Check Weighing

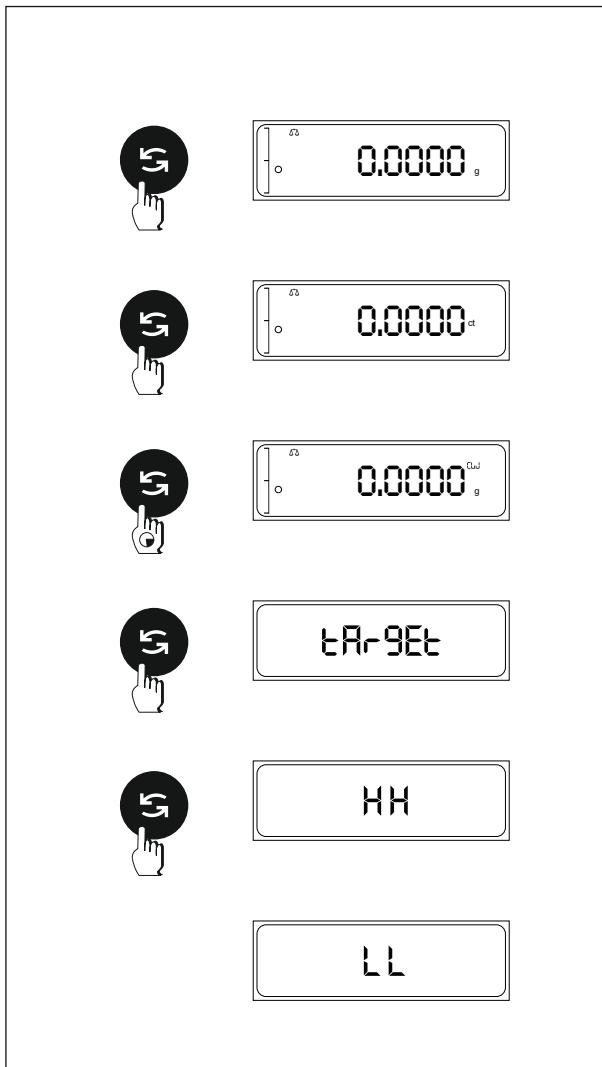

This feature is used to check whether a sample corresponds to a preset target or is within a specific tolerance range.

The results displayed can also be available on external port, which with the help of electronic processing can be used to control additional devices.


The check weighing procedure will always be carried out in unit 'gm'.

Check weighing presupposes that you have selected the 'F CHw' in the user menu.

### Procedure

- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until "CW" is displayed on the display.  
Your balance now needs the target and tolerance values.


If entering the check weighing for the first time the target and tolerance setting menu will be displayed.

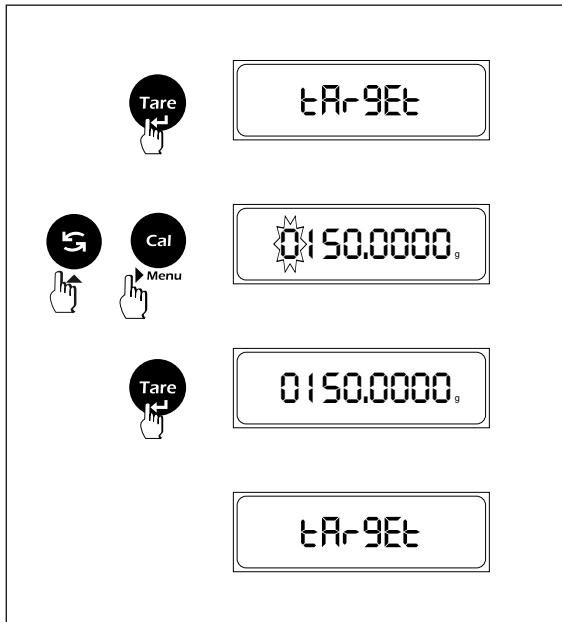

### Target and Tolerance Settings

- ⇒ Press and hold the <TOGGLE> until the target and tolerance setting menu is prompted.
- ⇒ Press the <TOGGLE> key to browse through the TARGET, HI, and LOW setting.
- ⇒ Press the <TARE> key to enter specific setting.
- ⇒ Press the <TOGGLE> key (▲) to change the value of the flashing digit.
- ⇒ Press the <CAL> key (►) to change the flashing digit from left to right.
- ⇒ After proper setting of values press the <TARE> key.
- ⇒ Press and hold the <TARE> key to store the values of target and tolerance values.

**Note:** To view the weight when the balance displays LL or HH press the <CAL> key press the <CAL> key again to display LL or HH.

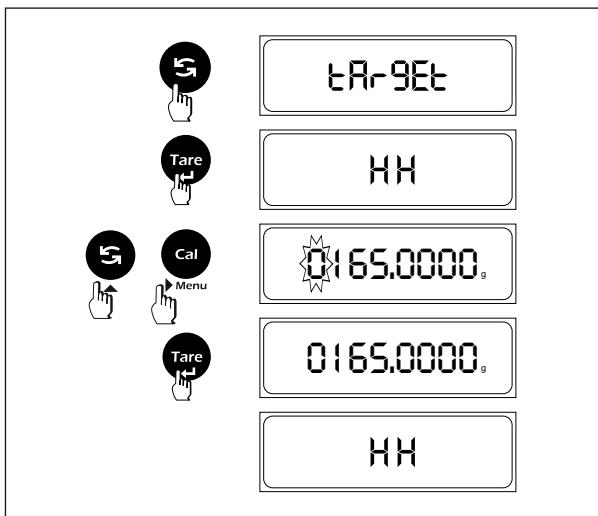

Load the weight on the pan and the balance will display the results according to the preset values of target and tolerance.

E.g. If the values are as follows,


TARGET = 150.0000 gm

HI = 155.0000 gm

LOW = 145.0000 gm

Now if 144.0000 gm is loaded on the pan the display shows LL indicating that the loaded weight is less than the low value set.

If 156.0000 gm is loaded on the pan the display shows HH indicating that the loaded weight is greater than the high value set.

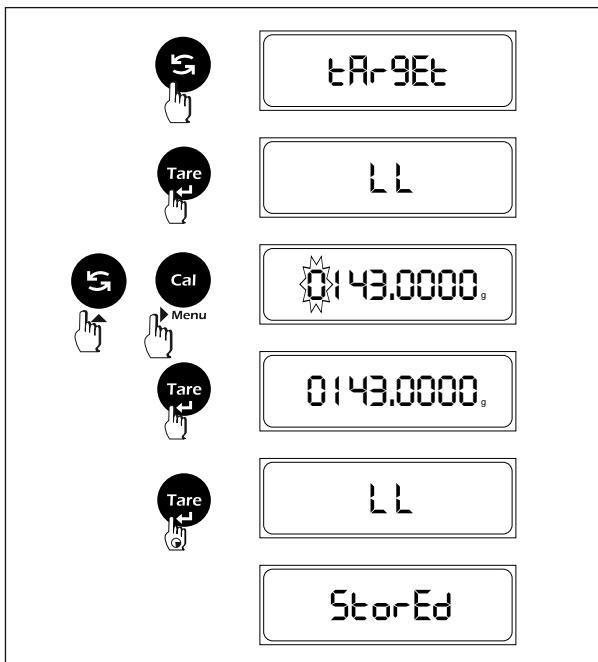

While the balance displays LL or HH the buzzer will beep continuously to indicate that the weight is out of the tolerance band and the corresponding lines on the external will be enabled.

If the weight is in the tolerance range the balance will display the weight similar to simple weighing.

You can use the <TOGGLE> key at any time to switch the display between check weighing, weighing unit 1 and weighing unit 2.

User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by CANCEL key and balance shows Current weights.

If the balance is connected eternally to PC or Printer through RS-232/USB then, whenever user enter into the Target and Tolerance Setting Menu of Check Weighing Menu & make changes in the setting, automatically printout is generated on the Peripheral attached.

In the printout, Target and Tolerance value are printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Chw**), Unit1 and Unit2 and Reference Weight is charged

|                |            |
|----------------|------------|
| Target         | 150.0000 g |
| Hi             | 160.0000 g |
| Lo             | 140.0000 g |
| ----- LL ----- |            |
| +              | 99.9979 g  |
| +              | 149.9979 g |
| ----- HH ----- |            |
| +              | 200.0029 g |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Chw**), Unit1 and Unit2 and Reference Weight is charged

|                         |            |
|-------------------------|------------|
| 05-Oct-23               | 10:35AM    |
| ----- ACZET -----       |            |
| Model                   | CY224C     |
| Ser.No.                 | 12345678   |
| Ver.No.                 | r.1.1.6.5  |
| Bal. ID.                | S/123      |
| -----                   |            |
| Product:                | XYZ        |
| Batch ID :              | T123       |
| Sample ID :             | L001       |
| Target                  | 150.0000 g |
| Hi                      | 160.0000 g |
| Lo                      | 100.0000 g |
| ----- LL -----          |            |
| +                       | 50.0515 g  |
| +                       | 50.0515 g  |
| ----- HH -----          |            |
| +                       | 200.0055 g |
| -----                   |            |
| 05-Oct-23               | 10:35AM    |
| ----- Signature : ----- |            |
| -----                   |            |


### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Chw**), Unit1 and Unit2 and Reference Weight is charged

|                                 |            |
|---------------------------------|------------|
| 05-Oct-23                       | 10:35AM    |
| ----- Aczet Mumbai, India ----- |            |
| Model                           | CY224C     |
| Ser.No.                         | 12345678   |
| Ver.No.                         | r.1.1.6.5  |
| Bal. ID.                        | S/123      |
| -----                           |            |
| Product:                        | XYZ        |
| Batch ID :                      | T123       |
| Sample ID :                     | L001       |
| Target                          | 170.0000 g |
| Hi                              | 190.0000 g |
| Lo                              | 110.0000 g |
| ----- LL -----                  |            |
| +                               | 50.0515 g  |
| ----- HH -----                  |            |
| +                               | 200.0055 g |
| -----                           |            |
| 05-Oct-23                       | 10:45AM    |
| ----- Signature : -----         |            |
| -----                           |            |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.

## 6.7 Totalization

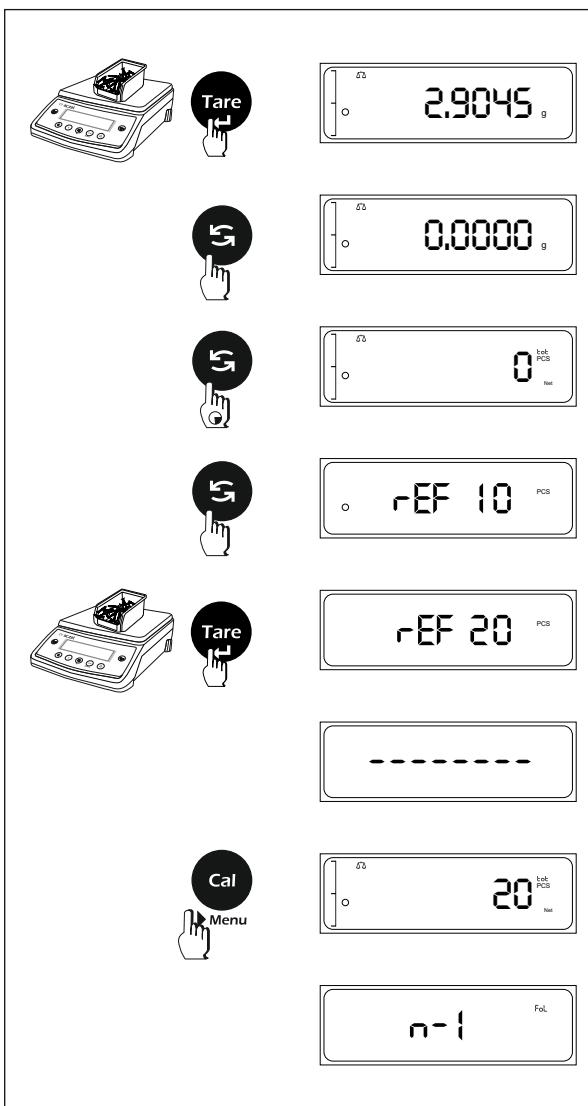

The totalization procedure allows individual weighing pieces to be summed to a total.

User can select from two available formulation modes i.e. Manual totalization and auto totalization.

Maximum no of weights that can be summed is 99.

Store component pieces with

- Display zeroed automatically after value is stored, and
- Automatic printout (print application parameters)
- Of the last added pieces and
- Of the total number of pieces.

Clear component memory when weighing series is canceled by pressing CANCEL key

**Note:**


- Individual weights can be added into summation only if the added pieces is greater than 2, this is indicated by "↓" symbol.

### 6.7.1 Manual Totalization

#### Procedure

Manual totalization presupposes that you have selected the 'F tot' in the user menu.

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until "tot" is displayed on the display.  
Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.

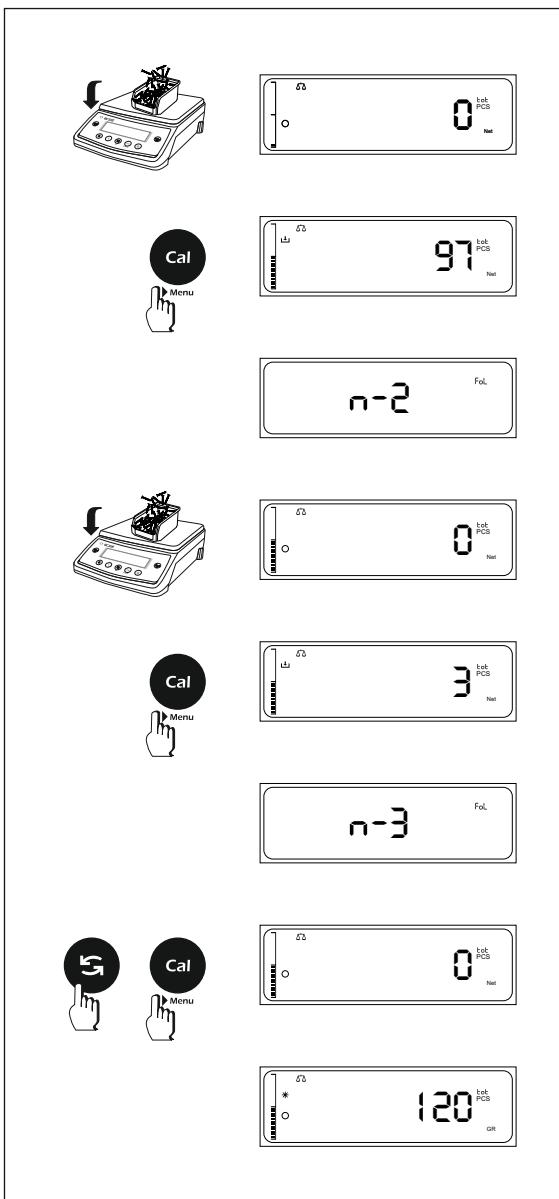

- ⇒ Your balance suggests the last set reference no. as the reference number. You can accept this suggestion or select one of the other reference numbers available (5, 10, 20, 50, 100 pieces) by briefly pressing the <TOGGLE> key.
- ⇒ Now place the selected number of reference pieces on the pan.
- ⇒ When you have placed exactly the same number of pieces on the weighing pan as selected reference pieces press TARE key.

As soon as the weighing result is stable, the calculated average piece weight is accepted as the reference.

- ⇒ Add weight on the pan. Weight can be added to summation when "↓" is displayed on the display i.e. when number of pieces is greater than 2.
- ⇒ Press the <CAL> key to store the weight, the balance displays "n-1" indicating that 1 weight is stored. The weight is tared automatically and simultaneously print command is given.

E.g. if 20.0000 gm and the reference is selected as 5, the printer output is as follows

nRef 5 pcs

wRef 4 g

N1 + 5 pcs

Tot + 5 pcs

Further addition of weights will give the following output (addition of 10.0000 gm).


N2 + 2 pcs

Tot + 7 pcs

- ⇒ To view the total weight, press the CAL and NEXT key together. The print command is given automatically

N 2

Tot + 7 pcs

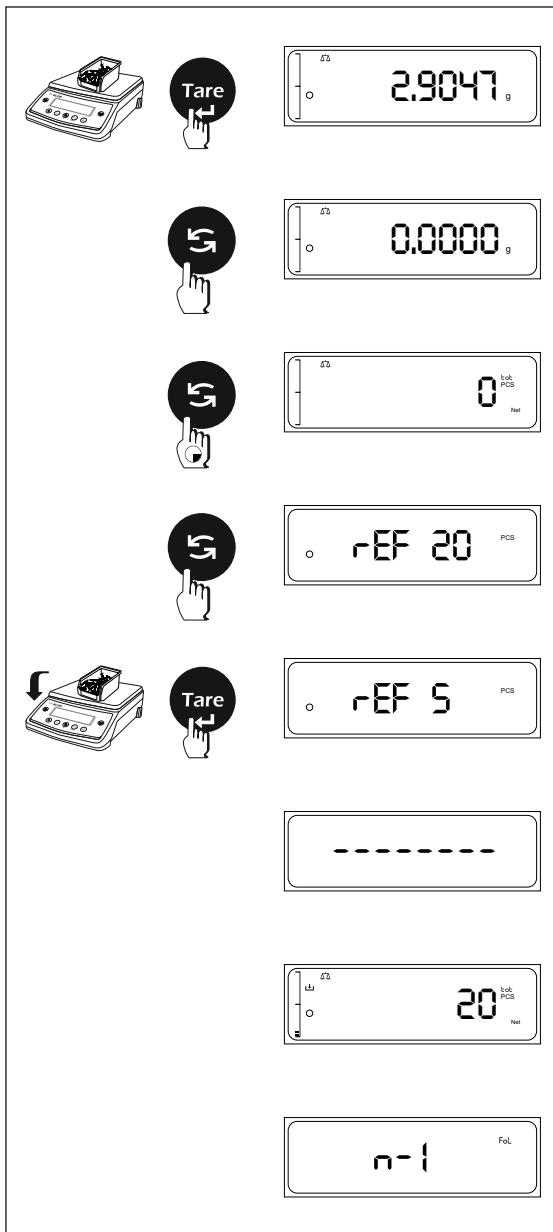


## 6.7.2 Auto Totalization

Auto totalization presupposes that you have selected the 'F tot AUTO' in the user menu. Auto totalization proves to be beneficial when the balance is used in majority **totalization** weighing and less for simple weighing thus reducing the time required for totalization as compared to **manualtotalization**

### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the <TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key briefly until “**tot**” and AUTO is displayed on the display. Your balance now needs the weight of a reference number.
- ⇒ Press and hold the <TOGGLE> key until you are prompted to load the reference pieces.
- ⇒ Your balance suggests the last selected reference number. You can accept this suggestion or select one of the other reference numbers available (5, 10, 20, 50, 100 pieces) by briefly pressing the <TOGGLE> key.
- ⇒ Now place the selected number of reference pieces on the pan.
- ⇒ When you have placed exactly the same number of pieces on the weighing pan as selected reference pieces press TARE key. As soon as the weighing result is stable, the calculated average piece weight is accepted as the reference.
- ⇒ Add weight on the pan. Weight can be added to summation when “” is displayed on the display i.e. when number of pieces is greater than 2.
- ⇒ When the weight is stable the number of pieces is stored in the totalization procedure and the balance displays “**n-1**” indicating that 1<sup>st</sup> weight is stored. The weight is tared automatically and simultaneously print command is given. Thus there is no need to press any to start the auto totalization procedure.

**Note :** You can use the <TOGGLE> key at any time to switch the display between totalization, weighing unit 1 and weighing unit 2. User can go to Standby mode by pressing on/off key and go to Simple Weighing with unit 1 by CANCEL key and balance shows Current weights.

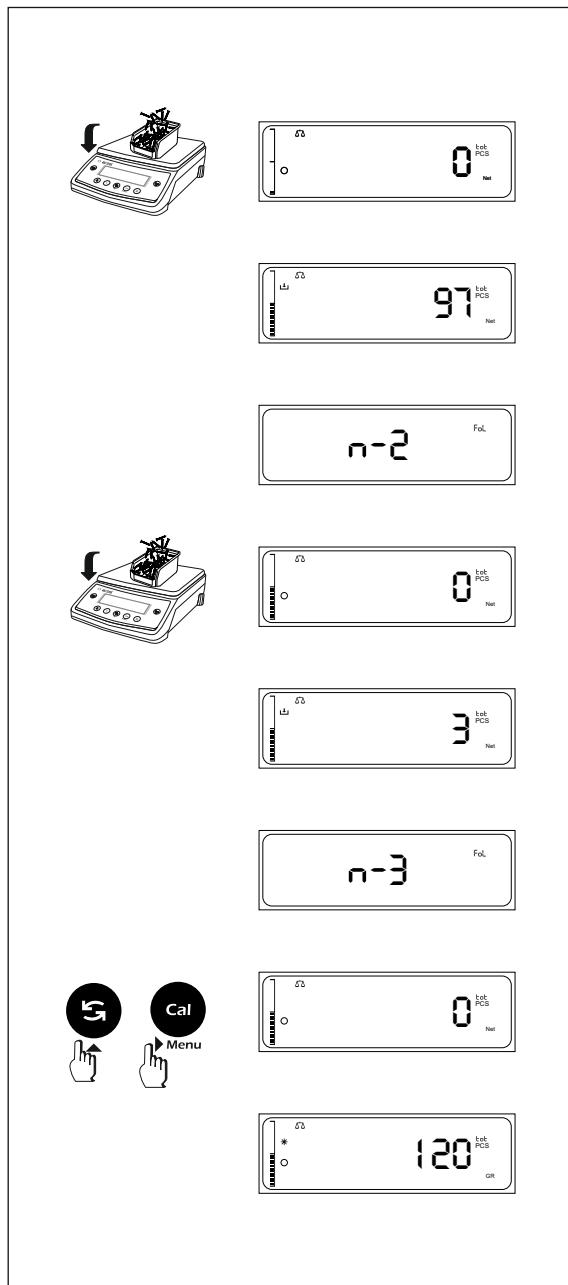

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the reference menu of Totalization function & make changes in the reference setting, automatically printout is generated on the Peripheral attached.

In the printout, reference number “nRef” and reference weight “wRef” is printed. After this user can Press Print Key to Print the reading on the display.

Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

#### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Tot**), Unit1 and Unit2 and Reference Weight is charged

|              |          |
|--------------|----------|
| <i>nRef</i>  | 10 pcs   |
| <i>wRef</i>  | 2.0000 g |
| <i>N1 +</i>  | 10 pcs   |
| <i>Tot +</i> | 10 pcs   |
| <i>N2 +</i>  | 25 pcs   |
| <i>Tot +</i> | 35 pcs   |
| <i>N3 +</i>  | 10 pcs   |
| <i>Tot +</i> | 45 pcs   |
| <i>N</i>     | 3        |
| <i>Tot +</i> | 45 pcs   |

#### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Tot**), Unit1 and Unit2 and Reference Weight is charged

|                    |           |
|--------------------|-----------|
| 05-Oct-23          | 10:35AM   |
| ACZET              |           |
| <i>Model</i>       | CY224C    |
| <i>Ser.No.</i>     | 12345678  |
| <i>Ver.No.</i>     | R.1.1.6.5 |
| <i>Bal. ID.</i>    | S/123     |
| <i>Product:</i>    | XYZ       |
| <i>Batch ID :</i>  | T123      |
| <i>Sample ID :</i> | L001      |
| <i>nRef</i>        | 20 pcs    |
| <i>wRef</i>        | 20 pcs    |
| <i>N1 +</i>        | 10 pcs    |
| <i>Tot +</i>       | 30 pcs    |
| <i>N2 +</i>        | 4 pcs     |
| <i>Tot +</i>       | 34 pcs    |
| <i>N3 +</i>        | 3         |
| <i>Tot +</i>       | 34 pcs    |
| <i>N</i>           |           |
| <i>Tot +</i>       | 10:35AM   |
| 05-Oct-23          |           |
| <i>Signature :</i> | .....     |

#### When Customize ON


Printouts generated when Unit Toggling is done between Application Unit (**Tot**), Unit1 and Unit2 and Reference Weight is charged

|                        |           |
|------------------------|-----------|
| 05-Oct-23              | 10:35AM   |
| Aczet<br>Mumbai, India |           |
| <i>Model</i>           | CY224C    |
| <i>Ser.No.</i>         | 12345678  |
| <i>Ver.No.</i>         | R.1.1.6.5 |
| <i>Bal. ID.</i>        | S/123     |
| <i>Product:</i>        | XYZ       |
| <i>Batch ID :</i>      | T123      |
| <i>Sample ID :</i>     | L001      |
| <i>nRef</i>            | 10 pcs    |
| <i>wRef</i>            | 5.0051 g  |
| <i>N1 +</i>            | 10 pcs    |
| <i>Tot +</i>           | 10 pcs    |
| <i>N2 +</i>            | 4 pcs     |
| <i>Tot +</i>           | 14 pcs    |
| <i>N</i>               | 2         |
| <i>Tot +</i>           | 14 pcs    |
| 05-Oct-23              | 10:45AM   |
| <i>Signature :</i>     | .....     |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.

2) To print footer user will have to Press <CANCEL> key.

## 6.8 Density Determination

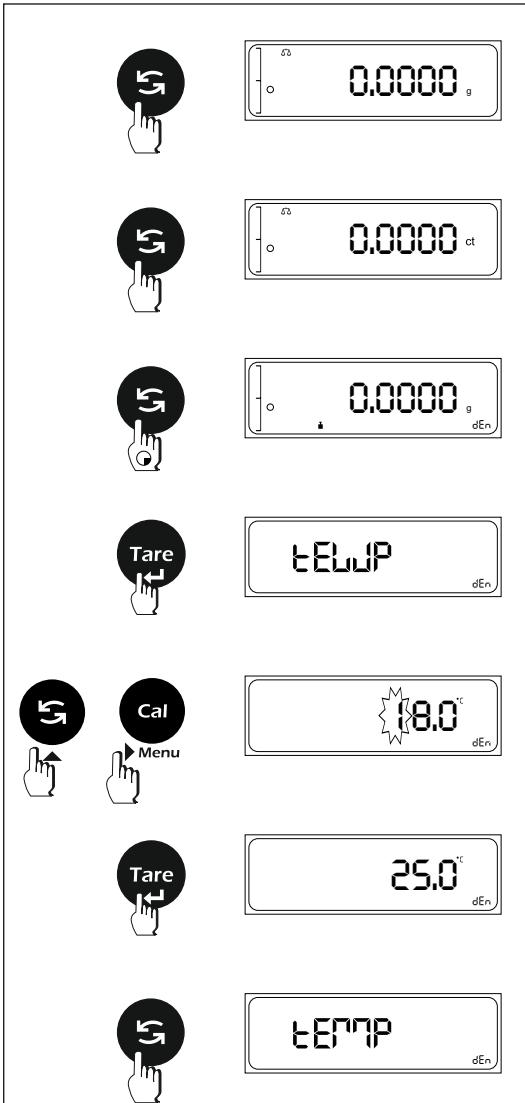

The density is determined applying the principle of Archimedes, which states that any body immersed in a fluid becomes lighter by an amount equal to the weight of the fluid that it has displaced.

Purity of gold can also be determined on the basis of density.

The weighing unit of density determination will be 'grams'.

Density determination presupposes that you have selected the 'F Den' in the user menu.


To calculate the density of sample, the balance should know the type of liquid and its temperature, used to calculate the density of solid.

### Procedure

- ⇒ Press and hold the <TOGGLE> until the functionality menu is prompted.
- ⇒ Press the <TOGGLE> key to browse through the Temperature, Liquid and Mode settings.

### Temperature Setting

- ⇒ Press the <TARE> key when the 'temp' is displayed.
- ⇒ Press the <TOGGLE> key (▲) to change the value of the flashing digit.
- ⇒ Press the <CAL> key (►) to change the flashing digit from left to right.
- ⇒ After proper setting of values press the <TARE> key.
- ⇒ The default value of temperature is **25.0°C**
- ⇒ This setting is alterable only when the liquid selected is water or ethanol. If the liquid selected is 'Other' the temperature setting will 'nA' i.e. Not applicable.

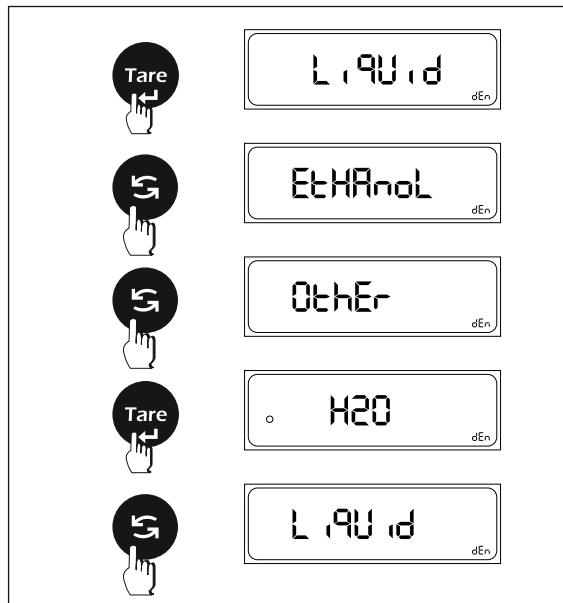


### Liquid Setting

You can select from the three available options i.e. water, ethanol and other.

- ⇒ Press the <TOGGLE> key to change the liquid option.
- ⇒ After proper selection of the liquid setting the <TARE> key.

The default option is distilled water.

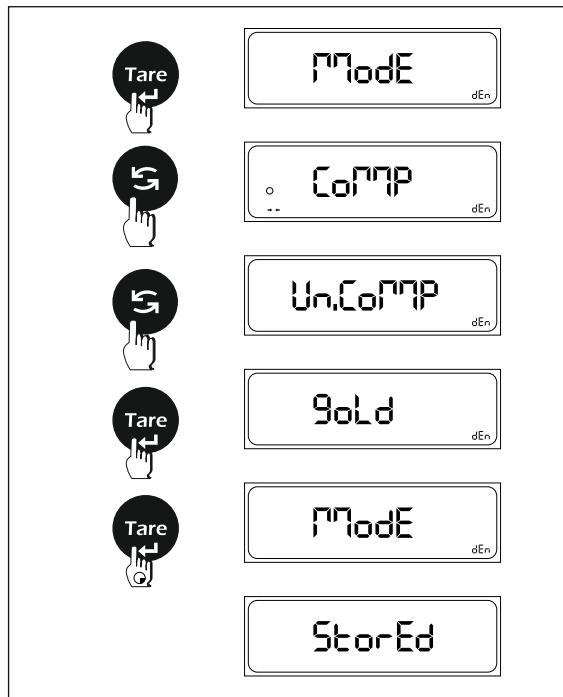


### Mode Setting

You can select from three options i.e. compensated, uncompensated and purity of gold.

- ⇒ Press the <TOGGLE> key to change the Mode setting.
- ⇒ After proper selection of mode press the <TARE> key .

The default option is compensated.

The results of purity of gold will be shown in carats.

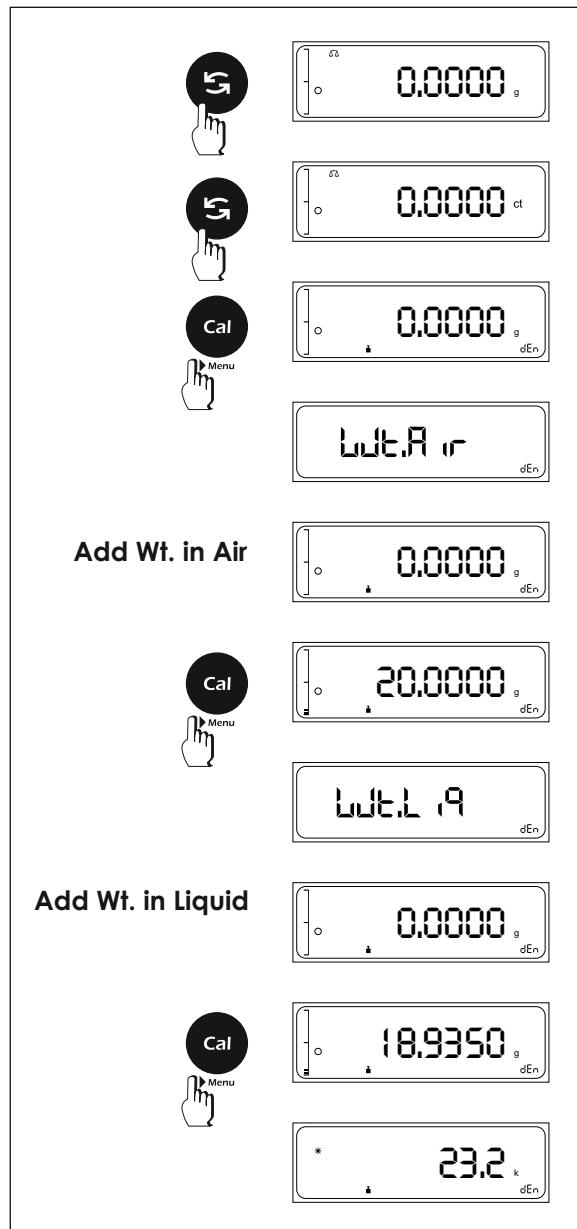

### Density Determination Procedure

- ⇒ Attach the Density determination Kit to the Balance
- ⇒ Press the <TARE> key briefly to TARE the balance.
- ⇒ Press the <TOGGLE> key briefly until "Den" appears on the display.
- ⇒ Press the <CAL> key to start the density determination procedure. The Balance now asks for weight of the sample in air. (With Wt.Air flashing on the display every 10 seconds)
- ⇒ Place the sample on density determination kit, When the weight is stable press the CAL key to accept the weight of sample in air.
- ⇒ Now the balance asks for the weight of sample in liquid (With Wt.Liqd flashing on the display every 10 seconds)
- ⇒ Now immerse the sample in the liquid, When the weight is stable press the CAL key to accept the weight of sample in liquid.
- ⇒ The balance will show the results upon the selected mode i.e. compensated, uncompensated or gold.

## Density Calculations

With compensation for air density

$$\tilde{n} = \frac{A * (\tilde{n}_0 - \tilde{n}_l)}{(A - B)} + \tilde{n}_l$$

$\tilde{n}$  = density of sample

A = weight of sample in air

B = weight of sample in auxiliary liquid

$\tilde{n}_0$  = density of auxiliary liquid

$\tilde{n}_l$  = air density (0.0012 g/cm<sup>3</sup>)

e.g.

$$\begin{aligned}\tilde{n} &= (A / (A - B)) (\tilde{n}_0 - \tilde{n}_l) + \tilde{n}_l \\ &= (20.000 / (20.000 - 18.935)) (0.99689 - 0.0012) + 0.0012 \\ &= 18.699 \text{ g/cm}^3\end{aligned}$$

Without compensation for air density


$$\tilde{n} = \frac{A}{(A - B)} * \tilde{n}_0$$

$$\tilde{n} = \tilde{n}_0 (A / (A - B))$$


e.g.

$$\begin{aligned}\tilde{n} &= \tilde{n}_0 (A / (A - B)) \\ &= (20.000 / (20.000 - 18.935)) (0.99689) \\ &= 18.721 \text{ g/cm}^3\end{aligned}$$

Display for compensated density

A digital display showing the value 18.699. Above the display is a small asterisk (\*). Below the display is a small 'dEn' label.

Display for uncompensated density

A digital display showing the value 18.721. Above the display is a small asterisk (\*). Below the display is a small 'dEn' label.

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Density function & make changes in the, automatically printout is generated on the Peripheral attached.

In the printout, Temperature, Liquid and Mode are printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Den**), Unit1 and Unit2 and Reference Weight is changed

|               |                  |
|---------------|------------------|
| <i>Mode</i>   | <i>GOLD</i>      |
| <i>Liquid</i> | <i>WATER</i>     |
| <i>Pur +</i>  | <i>23.1 ct</i>   |
| +             | <i>18.9350 g</i> |
| +             | <i>94.675 ct</i> |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Den**), Unit1 and Unit2 and Reference Weight is changed

|                    |                  |
|--------------------|------------------|
| <i>05-Oct-23</i>   | <i>10:35AM</i>   |
| <i>ACZET</i>       |                  |
| <i>Model</i>       | <i>CY224C</i>    |
| <i>Ser.No.</i>     | <i>12345678</i>  |
| <i>Ver.No.</i>     | <i>r.1.1.6.5</i> |
| <i>Bal. ID.</i>    | <i>S/123</i>     |
| <i>Product:</i>    | <i>XYZ</i>       |
| <i>Batch ID :</i>  | <i>T123</i>      |
| <i>Sample ID :</i> | <i>L001</i>      |
| <i>Mode</i>        | <i>GOLD</i>      |
| <i>Liquid</i>      | <i>WATER</i>     |
| <i>Pur +</i>       | <i>23.1 ct</i>   |
| +                  | <i>18.9350 g</i> |
| +                  | <i>94.675 ct</i> |
| <i>05-Oct-23</i>   | <i>10:35AM</i>   |
| <i>Signature :</i> | -----            |

### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Den**), Unit1 and Unit2 and Reference Weight is changed

|                      |                  |
|----------------------|------------------|
| <i>05-Oct-23</i>     | <i>10:35AM</i>   |
| <i>Aczet</i>         |                  |
| <i>Mumbai, India</i> |                  |
| <i>Model</i>         | <i>CY224C</i>    |
| <i>Ser.No.</i>       | <i>12345678</i>  |
| <i>Ver.No.</i>       | <i>r.1.1.6.5</i> |
| <i>Bal. ID.</i>      | <i>S/123</i>     |
| <i>Product:</i>      | <i>XYZ</i>       |
| <i>Batch ID :</i>    | <i>T123</i>      |
| <i>Sample ID :</i>   | <i>L001</i>      |
| <i>Mode</i>          | <i>GOLD</i>      |
| <i>Liquid</i>        | <i>WATER</i>     |
| <i>Pur +</i>         | <i>23.1 ct</i>   |
| +                    | <i>18.9350 g</i> |
| +                    | <i>94.675 ct</i> |
| <i>05-Oct-23</i>     | <i>10:35AM</i>   |
| <i>Signature :</i>   | -----            |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Density function & make changes in the, automatically printout is generated on the Peripheral attached.

In the printout, Temperature, Liquid and Mode are printed. After this user can Press Print Key to Print the reading on the display. Also user can Toggle to other unit through Toggle key & Press Print Key to get the print out of those corresponding units.

### When Standard ON

Printouts generated when Unit Toggling is done between Application Unit (**Den with Compensated Mode Liquid as Ethanol**), Unit1 and Unit2 and Reference Weight is changed

|             |             |
|-------------|-------------|
| Mode        | COMPENSATED |
| Liquid      | ETHANOL     |
| Tfemprature | 28.0        |
| Den +       | 0.6995 g/c3 |
| +           | 18.9350 g   |
| +           | 94.675 ct   |

### When GLP ON

Printouts generated when Unit Toggling is done between Application Unit (**Den with Compensated Mode Liquid as Ethanol**), Unit1 and Unit2 and Reference Weight is changed

|             |             |
|-------------|-------------|
| Model       | CY224C      |
| Ser.No.     | 12345678    |
| Ver.No.     | r.1.1.6.5   |
| Bal. ID.    | S/123       |
| Product:    | XYZ         |
| Batch ID :  | T123        |
| Sample ID : | L001        |
| Mode        | COMPENSATED |
| Liquid      | ETHANOL     |
| Tfemprature | 28.0        |
| Den +       | 0.6995 g/c3 |
| +           | 18.9350 g   |
| +           | 94.675 ct   |
| 05-Oct-23   | 10:35AM     |
| Signature : | -----       |


### When Customize ON

Printouts generated when Unit Toggling is done between Application Unit (**Den with Compensated Mode Liquid as Ethanol**), Unit1 and Unit2 and Reference Weight is changed

|             |             |
|-------------|-------------|
| Model       | CY224C      |
| Ser.No.     | 12345678    |
| Ver.No.     | r.1.1.6.5   |
| Bal. ID.    | S/123       |
| Product:    | XYZ         |
| Batch ID :  | T123        |
| Sample ID : | L001        |
| Mode        | COMPENSATED |
| Liquid      | ETHANOL     |
| Tfemprature | 28.0        |
| Den +       | 0.6995 g/c3 |
| +           | 18.9350 g   |
| +           | 94.675 ct   |
| 05-Oct-23   | 10:35AM     |
| Signature : | -----       |

**Note :** 1) User cannot enter into the external calibration or menu when GLP is ON & footer has not been printed.  
 2) To print footer user will have to Press <CANCEL> key.


## 6.9 Pipette Calibration

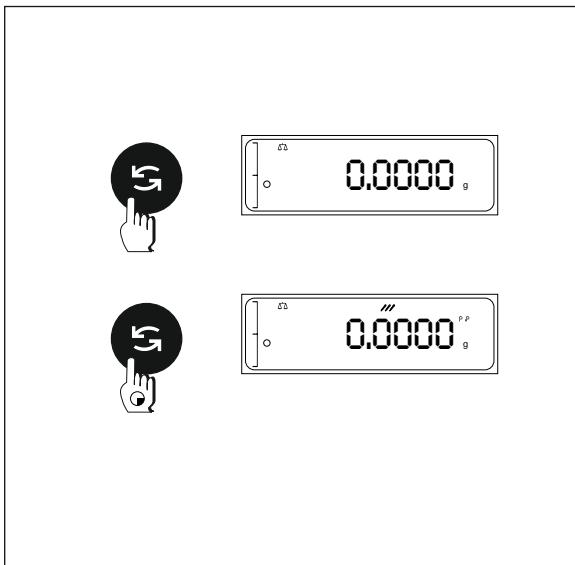

In laboratories, where pipettes are used for experimenting with liquids, it becomes important to calibrate the pipette. Thus this feature enables the user to calibrate the pipette. The feature "pipette calibration" can be activated by selecting the "F PiP" function in the menu. By pressing the CAL/MENU key for 4 seconds the user can enter the User menu and select the "F PiP" function.  
Note: The below procedure presupposes that you have selected the 'F PiP' function in the user menu.

### Procedure

- ⇒ Place the empty container on the pan.
- ⇒ Press the < TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key for 2 seconds to enter the F PiP function.

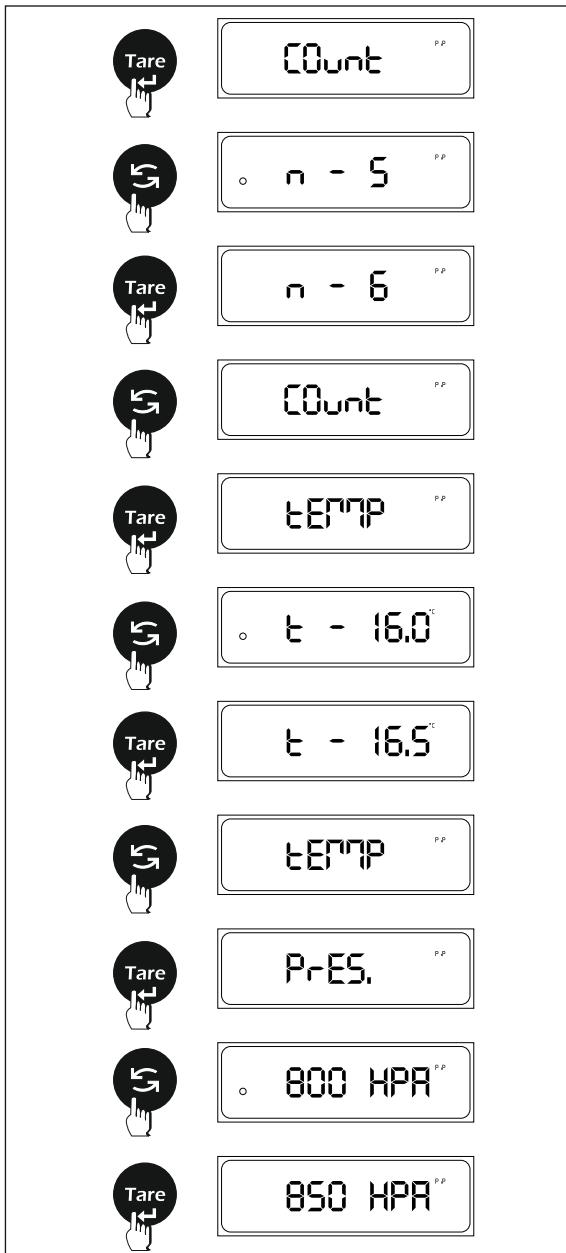

**Note:** To enter the settings below, it is assumed that the user has already performed the above procedure and the scale is in F PiP mode.

### Count Cycle Settings


- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Press < TARE> to enter the count settings.
- ⇒ 'n' represents the number of calibration cycles the user intends to perform. 'n' can have any value between 5 and 15 (including both).
- ⇒ Press <TOGGLE> to select the required value of 'n'.
- ⇒ Press <TARE> once to select the value of 'n' and return to F PiP settings.
- ⇒ The default count value is 5.

### Temperature settings

- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Select 'tEMP' in F PiP settings by pressing <TOGGLE> key.
- ⇒ Press < TARE> to enter the 'tEMP' settings.
- ⇒ The user can select from a list of 30 predefined temperatures ranging from 15.0°C to 30.0°C with a step interval of 0.5°C.
- ⇒ Change the temperature value by pressing <TOGGLE> key and then select it pressing <TARE>. This will bring you back to F PiP settings.
- ⇒ The default temperature is 25.0°C

### Pressure Settings

- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Select 'PrES' in F PiP settings by pressing <TOGGLE> key.
- ⇒ Press < TARE> to enter the 'PrES' settings.
- ⇒ The user can select from a list of 7 predefined pressures ranging from 800 hPa to 1050 hPa with step interval of 50 hPa.
- ⇒ Change the pressure value by pressing the <TOGGLE> key and then select it pressing <TARE>. This will bring you back to 'FPiP' settings.
- ⇒ The default pressure is 800 hPa.

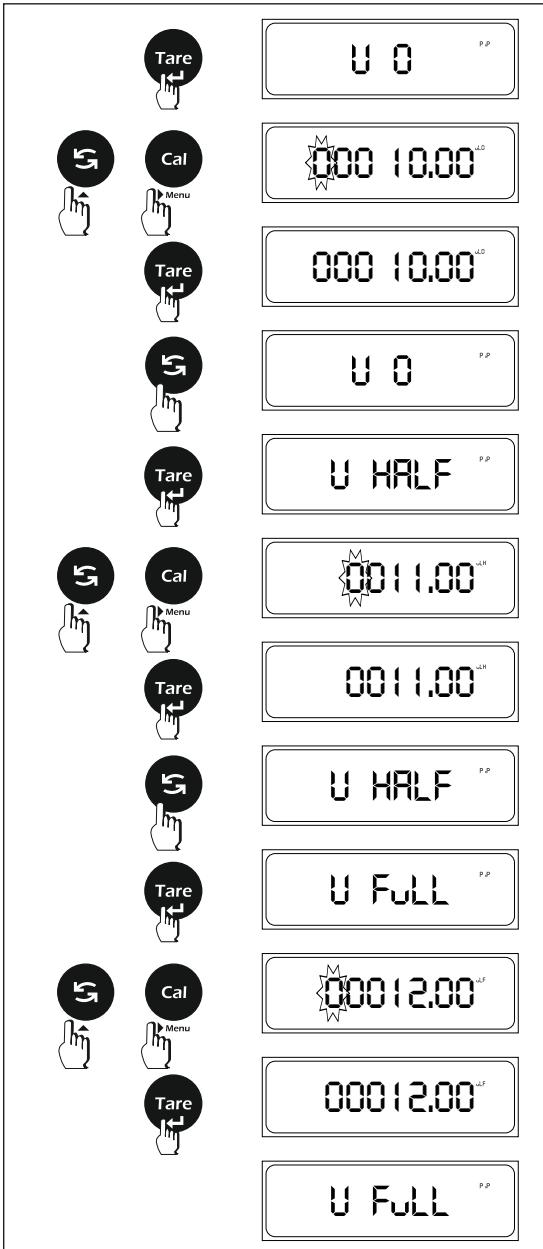

## Volume Settings:

### Initial volume $V_0$ :


- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Select ' $V_0$ ' in F PiP settings by pressing <TOGGLE> key.
- ⇒ Press < TARE> to enter the ' $V_0$ ' settings.
- ⇒ The user can change the volume with the help of <CAL/MENU> key and <TOGGLE>key.
- ⇒ Pressing the <CAL/MENU> key will shift the cursor to the right in a cyclic way and pressing the <TOGGLE> key will increment the digit.
- ⇒ Press the <TARE> key to select the value. This will bring you back to the F PiP menu
- ⇒ The default volume is,  $V_0 = 10.00 \mu\text{L}$

### Half volume $V_{\text{Half}}$ :

- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Select ' $V_{\text{Half}}$ ' in F PiP settings by pressing <TOGGLE> key.
- ⇒ Press < TARE> to enter the ' $V_{\text{Half}}$ ' settings.
- ⇒ The user can change the volume with the help of <CAL/MENU> key and <TOGGLE>key.
- ⇒ Pressing the <CAL/MENU> key will shift the cursor right in a cyclic way and pressing the <TOGGLE> key will increment the digit.
- ⇒ Press the <TARE> key to select the value. This will bring you back to the F PiP menu
- ⇒ The default volume is,  $V_{\text{Half}} = 11.00 \mu\text{L}$

### Full volume, $V_{\text{Full}}$ :

- ⇒ Press <TOGGLE> key to enter F PiP settings.
- ⇒ Select ' $V_{\text{Full}}$ ' in F PiP settings by pressing <TOGGLE> key.
- ⇒ Press < TARE> to enter the ' $V_{\text{Full}}$ ' settings.
- ⇒ The user can change the volume with the help of <CAL/MENU> key and <TOGGLE>key.
- ⇒ Pressing the <CAL/MENU> key will shift the cursor right in a cyclic way and pressing the <TOGGLE> key will increment the digit.
- ⇒ Press the <TARE> key to select the value. This will bring you back to the F PiP menu
- ⇒ The default volume is,  $V_{\text{Full}} = 12.00 \mu\text{L}$

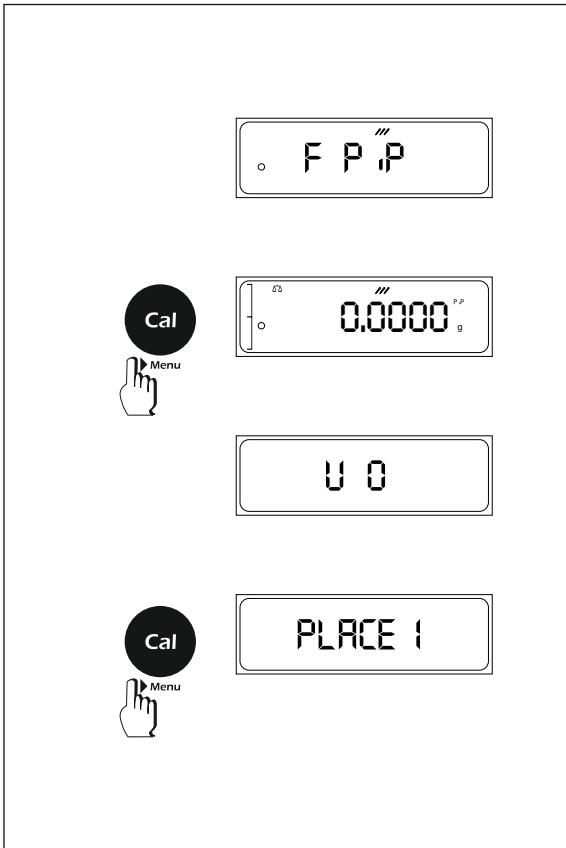

### Note:

- ⇒ It is assumed that the user has already performed the above procedure and the scale is in F PiP mode.
- ⇒ When the pipette calibration procedure process has not started the system will perform normal weighing with the unit as gm.

### Calibration procedure:

- ⇒ The calibration procedure repeats itself 'n' times where 'n' is the count entered in the count cycle settings (in FPiP settings).
- ⇒ Once in F PiP mode, press the <CAL/MENU> key to start the calibration process.
- ⇒ Once the <MENU/CAL> key is pressed, it will ask for the initial volume  $V_0$ .
- ⇒ For a calibration procedure of 'n' times, the scale will ask for  $V_0$  'n' times. Each of these value will be stored as 'PLACE n'.
- ⇒ Thus, for the 1<sup>st</sup> time, place the initial volume and press <CAL/MENU> key once the stability is achieved. This is accepted as 'PLACE 1'.
- ⇒ Follow the above procedure for 'PLACE 1' to 'PLACE n'.
- ⇒ Repeat the above procedure for half volume  $V_{\text{half}}$  and full volume  $V_{\text{full}}$  each 'n' times respectively.
- ⇒ In case of a successful calibration the scale will display 'PiP done'. If not, then it will ask to repeat the step wrongly performed.

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Pipette Calibration & make changes in it, automatically printout is generated on the Peripheral attached.

The following are the parameters that are Printed along with the readings :

### When GLP ON

|           |         |                    |                     |  |
|-----------|---------|--------------------|---------------------|--|
| 05-Oct-23 | 10:35AM | Results :          | V1/2                | Legend   |
|           |         | 1                  | 20029.28 <i>uL</i>  | V <sub>a</sub> : <i>Mean Value</i>                                     |
|           |         | 2                  | 0.00 <i>uL</i>      | E <sub>s</sub> : <i>Systematic Error</i>                               |
|           |         | 3                  | 20029.38 <i>uL</i>  | E <sub>s%</sub> : <i>E<sub>s</sub> expressed as % of nominal value</i> |
|           |         | 4                  | 70189.50 <i>uL</i>  |  |
|           |         | 5                  | 70189.30 <i>uL</i>  |  |
|           |         | V1/2 =             | 12.00 <i>uL</i>     | S <sub>r</sub> : <i>Standard Deviation</i>                             |
|           |         | V <sub>a</sub> =   | 36087.49 <i>uL</i>  | C <sub>V</sub> : <i>Coefficient of Variation</i>                       |
|           |         | E <sub>s</sub> =   | 36075.49 <i>uL</i>  |  |
|           |         | E <sub>s%</sub> =  | 300629.08 %         | 05-Oct-23 10:35AM  |
|           |         | S <sub>r</sub> =   | 32186.63 <i>uL</i>  | Signature :  |
|           |         | C <sub>V</sub> =   | 89.19 %             |  |
| <hr/>     |         |                    |                     |  |
|           |         | Results :          | V <sub>max</sub>    |  |
|           |         | 1                  | 97306.56 <i>uL</i>  |  |
|           |         | 2                  | 97306.56 <i>uL</i>  |  |
|           |         | 3                  | 147500.35 <i>uL</i> |  |
|           |         | 4                  | 167555.78 <i>uL</i> |  |
|           |         | 5                  | 167555.78 <i>uL</i> |  |
|           |         | V <sub>max</sub> = | 13.00 <i>uL</i>     |  |
|           |         | V <sub>a</sub> =   | 135445.01 <i>uL</i> |  |
|           |         | E <sub>s</sub> =   | 135432.01 <i>uL</i> |  |
|           |         | E <sub>s%</sub> =  | 1041784.67 %        |  |
|           |         | S <sub>r</sub> =   | 35765.26 <i>uL</i>  |  |
|           |         | C <sub>V</sub> =   | 26.41 %             |  |
| <hr/>     |         |                    |                     |  |

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Pipette Calibration & make changes in it, automatically printout is generated on the Peripheral attached.

The following are the parameters that are Printed along with the readings :

## When Customize ON

|                      |                    |                    |                     |   |
|----------------------|--------------------|--------------------|---------------------|---|
| 05-Oct-23            | 10:35AM            | Results :          | V1/2                | Legend  |
|                      |                    | 1                  | 70190.00 <i>uL</i>  | V <sub>a</sub> : Mean Value                     |
| Aczet                |                    | 2                  | 70190.00 <i>uL</i>  | E <sub>s</sub> : Systematic Error               |
| Mumbai, India        |                    | 3                  | 50152.20 <i>uL</i>  | E <sub>s%</sub> : E <sub>s</sub> expressed as % |
| Model                | CY224C             | 4                  | 70190.00 <i>uL</i>  | of nominal value                                |
| Ser.No.              | 12345678           | 5                  | 70190.00 <i>uL</i>  |   |
| Ver.No.              | r.1.1.6.5          | V1/2 =             | 12.00 <i>uL</i>     | S <sub>r</sub> : Standard Deviation             |
| Bal. ID.             | S/123              | V <sub>a</sub> =   | 66182.44 <i>uL</i>  | C <sub>V</sub> : Coefficient of                 |
| Product :            | XYZ                | E <sub>s</sub> =   | 66170.44 <i>uL</i>  | Variation                                       |
| Batch ID :           | T123               | E <sub>s%</sub> =  | 551420.33 %         |   |
| Sample ID :          | L001               | S <sub>r</sub> =   | 8961.17 <i>uL</i>   | 05-Oct-23 10:35AM                               |
| PIPETTE CAL. RESULTS |                    | CV =               | 13.54 %             | Signature : -----                               |
| Count :              | 5 Cnt              | Results :          | V <sub>max</sub>    |   |
| Temp. :              | 16.0{C° C          | 1                  | 97307.06 <i>uL</i>  |   |
| Pressure :           | 900 hPa            | 2                  | 97307.06 <i>uL</i>  |   |
| Results :            | V <sub>min</sub>   | 3                  | 117352.88 <i>uL</i> |   |
| 1                    | 20029.58 <i>uL</i> | 4                  | 117352.88 <i>uL</i> |   |
| 2                    | 20029.48 <i>uL</i> | 5                  | 167556.98 <i>uL</i> |   |
| 3                    | 50152.30 <i>uL</i> | V <sub>max</sub> = | 13.00 <i>uL</i>     |   |
| 4                    | 20029.68 <i>uL</i> | V <sub>a</sub> =   | 119375.37 <i>uL</i> |   |
| 5                    | 20029.68 <i>uL</i> | E <sub>s</sub> =   | 119362.37 <i>uL</i> |   |
| V <sub>min</sub> =   | 11.00 <i>uL</i>    | E <sub>s%</sub> =  | 918172.09 %         |   |
| V <sub>a</sub> =     | 26054.14 <i>uL</i> | S <sub>r</sub> =   | 28738.78 <i>uL</i>  |   |
| E <sub>s</sub> =     | 26043.14 <i>uL</i> | CV =               | 24.07 %             |   |
| E <sub>s%</sub> =    | 236755.85 %        |                    |                     |   |
| S <sub>r</sub> =     | 13471.28 <i>uL</i> |                    |                     |   |
| CV =                 | 51.70 %            |                    |                     |   |

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Pipette Calibration & make changes in it, automatically printout is generated on the Peripheral attached.

The following are the parameters that are Printed along with the readings :

## When Standard ON

### PIPETTE CAL. RESULTS


Count : 5 Cnt  
 Temp. : 16.0°C  
 Pressure : 900 hPa  
 Results : Vmin  
 1 20029.58 uL  
 2 20029.48 uL  
 3 50152.30 uL  
 4 20029.68 uL  
 5 20029.68 uL  
 Vmin = 11.00 uL  
 Va = 26054.14 uL  
 Es = 26043.14 uL  
 Es% = 236755.85 %  
 Sr = 13471.28 uL  
 CV = 51.70 %  
 -----

Results : V1/2  
 1 70190.00 uL  
 2 70190.00 uL  
 3 50152.20 uL  
 4 70190.00 uL  
 5 70190.00 uL  
 V1/2 = 12.00 uL  
 Va = 66182.44 uL  
 Es = 66170.44 uL  
 Es% = 551420.33 %  
 Sr = 8961.17 uL  
 CV = 13.54 %  
 -----  
 Results : Vmax  
 1 97307.06 uL  
 2 97307.06 uL  
 3 117352.88 uL  
 4 117352.88 uL  
 5 167556.98 uL  
 Vmax = 13.00 uL  
 Va = 119375.37 uL  
 Es = 119362.37 uL  
 Es% = 918172.09 %  
 Sr = 28738.78 uL  
 CV = 24.07 %  
 -----

### Legend

Va : Mean Value  
 Es : Systematic Error  
 Es% : Es expressed as % of nominal value  
 Sr : Standard Deviation  
 CV : Coefficient of Variation  
 -----

## 6.10 Statistics

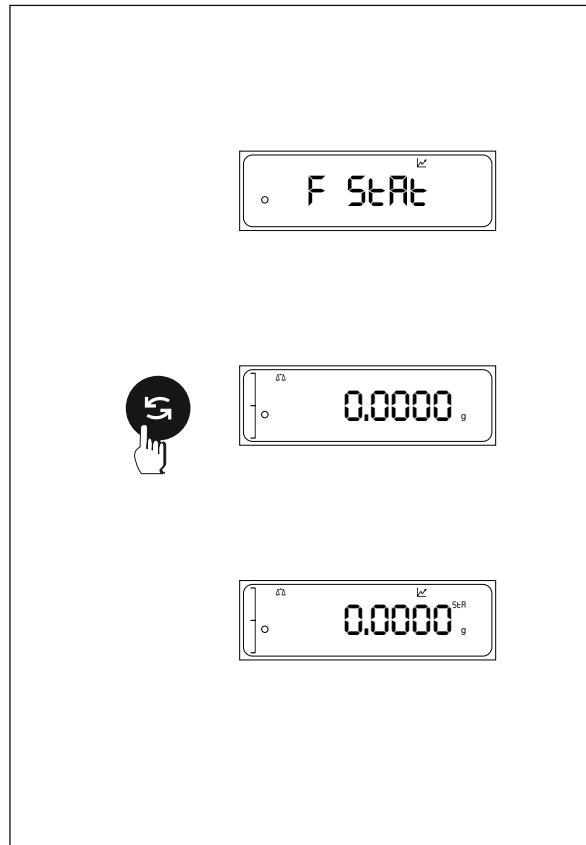


With this feature, the user can obtain the statistics of the data stored in the scale. These statistics includes the details such as number of readings 'n', Average, Minimum value, Maximum value, Standard deviation, Difference and Co efficient of Variance. The feature 'F STAT' can be activated by selecting the 'F STAT' function in the menu. This can be done by pressing the <CAL/MENU> key for 4 seconds and changing the feature by <TOGGLE> key. Press <TARE> key to select 'F STAT'. press <TARE> for 2 seconds to store the selection.

The below procedure presupposes that you have selected the 'F STAT' function in the user menu.

### Procedure


- ⇒ Place the empty container on the pan.
- ⇒ Press the < TARE> key briefly to tare the balance.
- ⇒ Press the <TOGGLE> key for entering the 'F STAT' function.

**Note:** To use the 'F STAT' function, it is assumed that the user has already performed the above procedure and the scale is in 'F STAT' mode.

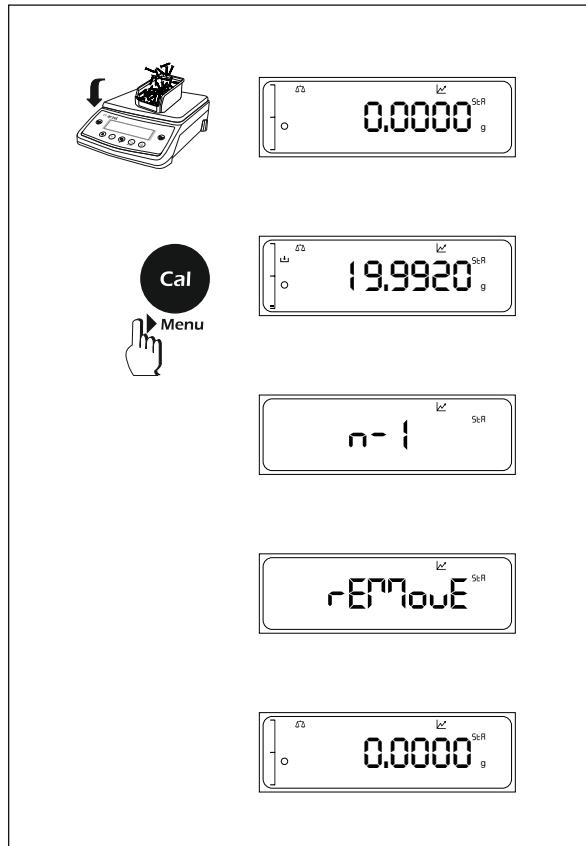

## Statistics procedure

- ⇒ The user can now place weight on the pan and press the <CAL/MENU> key once the stability is achieved.
- ⇒ The scale should display 'n-1' (where 'n' is the number of the current weight) and will retain this as first weight.
- ⇒ "rmv" will be displayed on screen for 2 seconds to instruct the user to unload the weight.
- ⇒ The next weight will be taken into statistics only after user has taken off the weight from the pan, such that the weight on the pan should now be 0.0000g.
- ⇒ Repeat the above procedure for rest of the data entries.

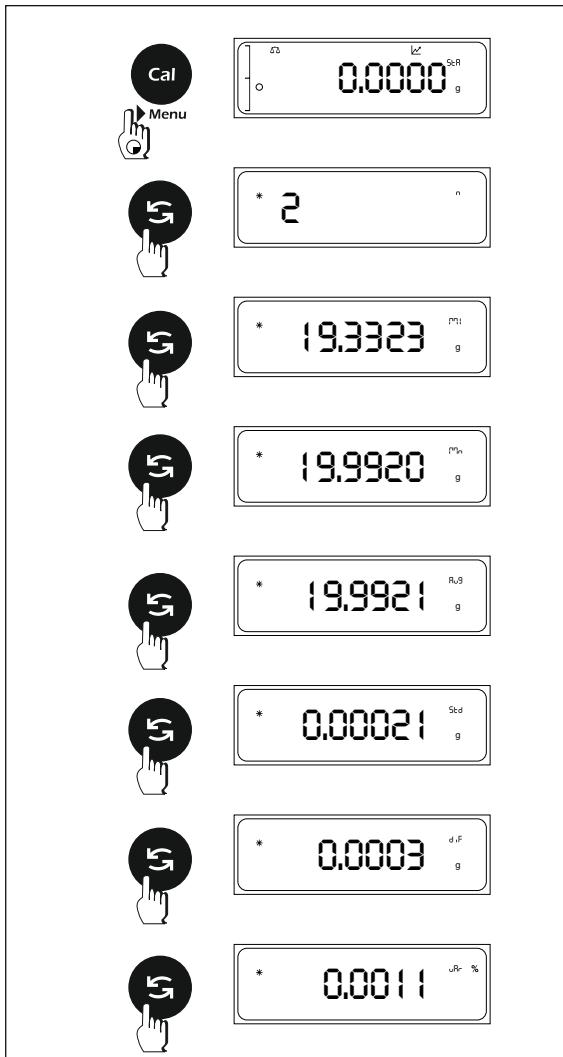

## Reading the statistics

- ⇒ At any point of time, the user can press and hold the <TOGGLE> key for 2 seconds to go through the statistics.
- ⇒ The screen will display the 1<sup>st</sup> parameter as number of readings 'n' along with the star symbol which indicates that the user is in the statistics result mode.
- ⇒ The user can now go through the other parameters such as average, Min value, Max value, Standard deviation, Difference, Co efficient of Variance by pressing the <TOGGLE> key.
- ⇒ The user can come out of the statistics mode by pressing the < CANCEL > key.

## Deleting statistics:

- ⇒ The user can delete the statistics by pressing the <TARE> key for 2 seconds when in 'StAt' mode.
- ⇒ This will delete the previous data entries and start again.
- ⇒ The entire data is will be sent to the terminal or to the printer before it gets deleted.

## Note:

- ⇒ The minimum weight on the pan should be 10d (where 'd' is the accuracy of the scale), if less than that, then the weight will not be taken into consideration for calculating statistics.
- ⇒ The statistics will be deleted if the system goes into standby mode (i.e. if the auto-off feature is active or by power on-off).
- ⇒ The user can also print the statistics by pressing the <PRINT> key when in 'StAt' mode.

If the balance is connected externally to PC or Printer through RS-232/USB then, whenever user enter into the menu of Statistics & presses in the print key , the user can obtain the list of parameters shown in the below example :

### When Standard ON

|       |          |
|-------|----------|
| 001 + | 1.5750 g |
| 002 + | 2.3500 g |
| 003 + | 7.8950 g |
| 004 + | 4.1750 g |
| ----- |          |
| N     | 4        |
| MAX   | 7.8950 g |
| MIN   | 1.5750 g |
| AVG   | 3.9987   |
| STD   | 2.8169   |
| VAR   | 7.9349   |
| ----- |          |



### When GLP ON

|             |            |
|-------------|------------|
| 05-Oct-23   | 10:35AM    |
| -----       |            |
| ACZET       |            |
| Model       | CY224C     |
| Ser.No.     | 12345678   |
| Ver.No.     | r.1.1.6.5  |
| Bal. ID.    | S/123      |
| -----       |            |
| Product :   | XYZ        |
| Batch ID :  | T123       |
| Sample ID : | L001       |
| 001 +       | 97.1118 g  |
| 002 +       | 19.9893 g  |
| 003 +       | 200.0028 g |
| 004 +       | 50.0509 g  |
| -----       |            |
| N           | 4          |
| MAX         | 200.0028 g |
| MIN         | 19.9893 g  |
| AVG         | 91.7887 g  |
| STD         | 91.7887 g  |
| DIF         | 180.0135 g |
| VAR         | 85.8666 %  |
| -----       |            |
| 05-Oct-23   | 10:35AM    |
| Signature : | -----      |
| -----       |            |

### When Customize ON

|               |            |
|---------------|------------|
| 05-Oct-23     | 10:35AM    |
| -----         |            |
| Aczet         |            |
| Mumbai, India |            |
| Model         | CY224C     |
| Ser.No.       | 12345678   |
| Ver.No.       | r.1.1.6.5  |
| Bal. ID.      | S/123      |
| -----         |            |
| Product :     | XYZ        |
| Batch ID :    | T123       |
| Sample ID :   | L001       |
| 001 +         | 200.0040 g |
| 002 +         | 50.0510 g  |
| 003 +         | 97.1113 g  |
| 004 +         | 19.9892 g  |
| -----         |            |
| N             | 4          |
| MAX           | 200.0040 g |
| MIN           | 19.9892 g  |
| AVG           | 91.7889 g  |
| STD           | 78.8164 g  |
| DIF           | 180.0148 g |
| VAR           | 85.8671 %  |
| -----         |            |
| 05-Oct-23     | 10:35AM    |
| Signature :   | -----      |
| -----         |            |


## Key Functionality in parameter settings mode



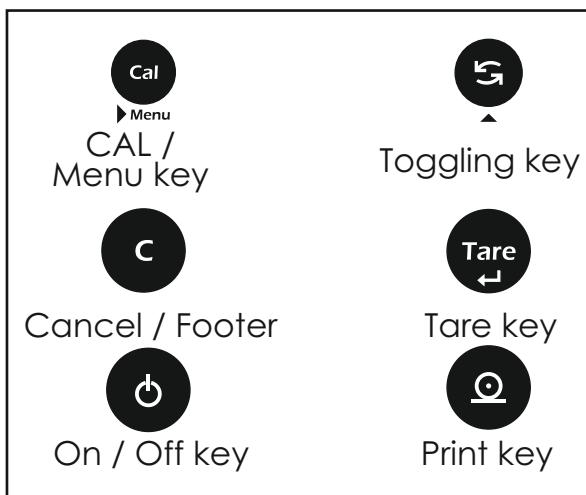
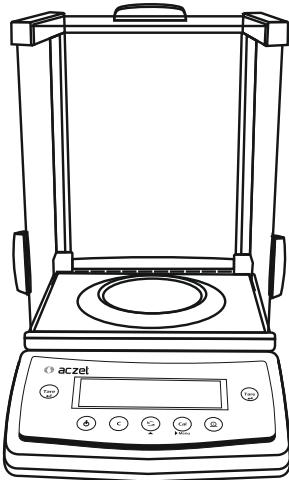


## 7. Parameter Settings

The following section explains key functionality in parameter settings mode.

| Press briefly   | Press & Hold                        |
|---|-------------------------------------|
| Change Sub Menu Setting<br>Increments the value of digit        |                                     |
| Change Main menu options<br>Shifts the digit from left to right |                                     |
| Confirm Setting   | Store and quit menu (Auto Cal Menu) |
| To Change Time Format (AM / PM / 24 hours) in Time Settings     |                                     |
| Quit the Current Parameter Menu                                 |                                     |

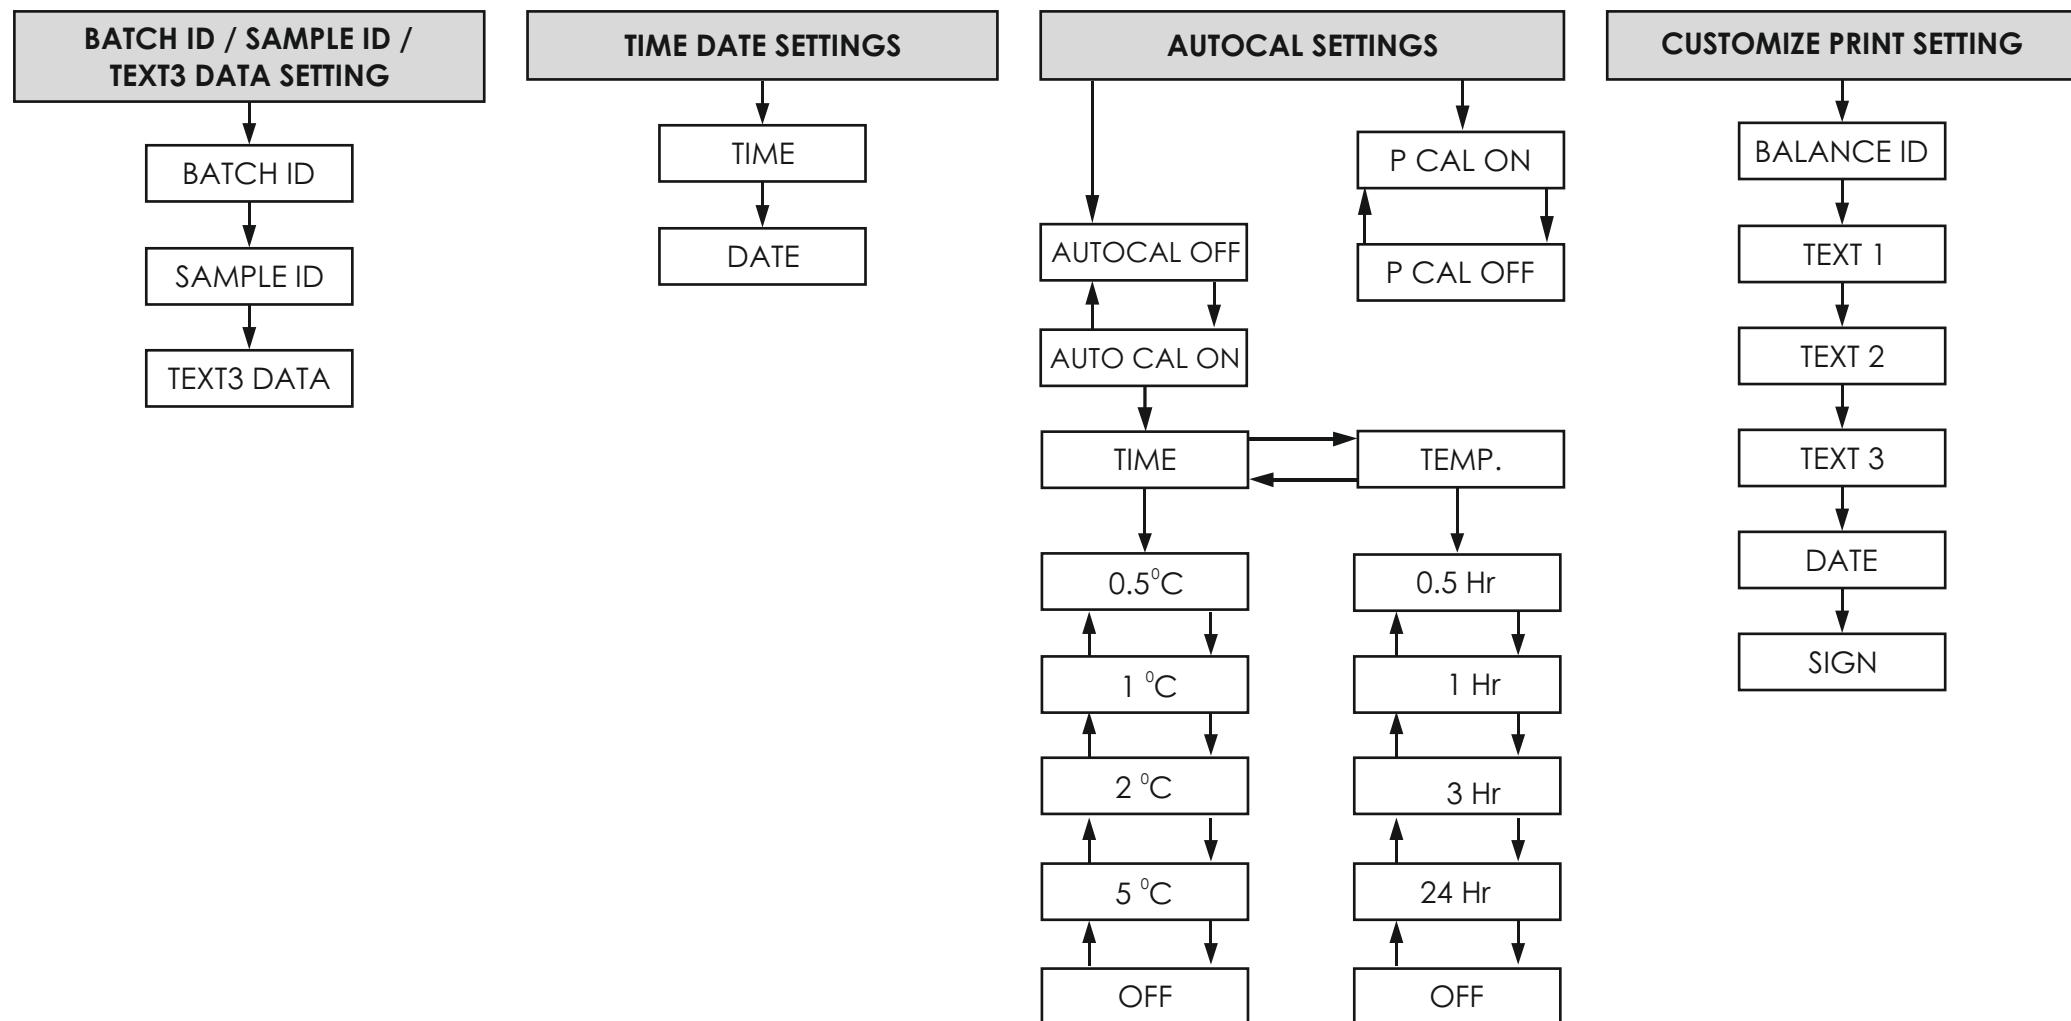

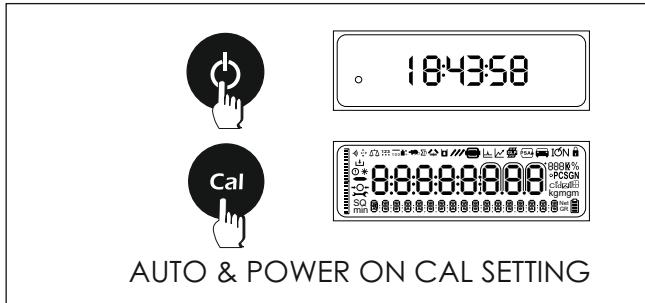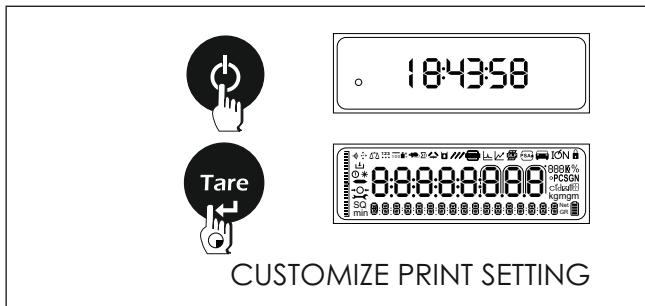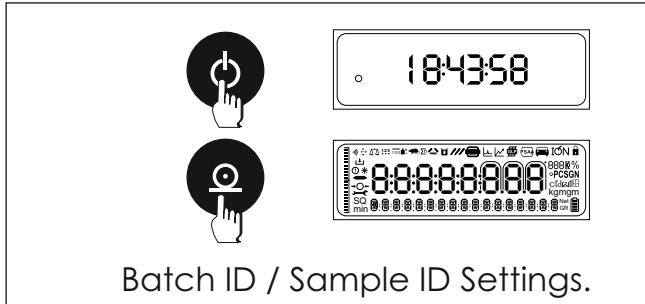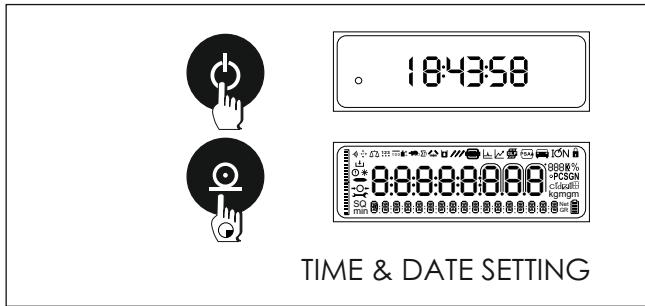

## Parameter Setting


By accessing the parameter menus the user can change the following settings.

- Time and Date Settings.
- Batch ID / Sample ID Settings.
- Customize Print Settings.
- Auto Calibration and Power On Calibration Settings.

## Operating Instructions

These menus can be accessed by pressing the PRINT key or CAL key or TARE key when all the characters of the display when coming out of stand by mode or Power On.

## 7.1 Time & Date Setting

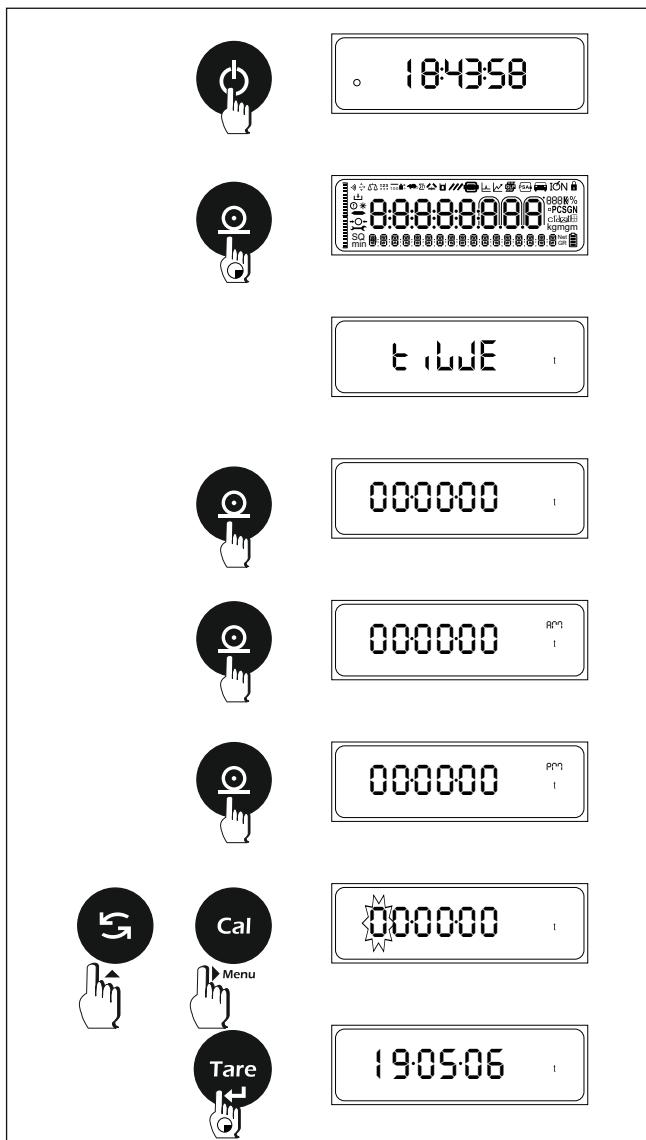

In this menu, User can set the Clock.

Clock setting consist of 2 settings. They are

TIME : In this submenu user can set the time in hours, minutes & seconds AM, PM & 24 hrs.


DATE : In this submenu user can set the date, Month & Years

### Operating Instructions

⇒ Press the PRINT key for 2 sec when coming out from stand by or Power on mode.

#### 7.1.1 SET TIME


⇒ Current Time is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.  
⇒ Press TOGGLE key ( ▲ ) to change the value of the Flashing digit.  
⇒ Press CAL key ( ► ) to shift the flashing digit from Left to Right  
⇒ After proper setting of time in hours, minutes & seconds respectively for zeroes starting from left, press Tare key  
⇒ Press the PRINT key to Change the format AM, PM & 24hrs.

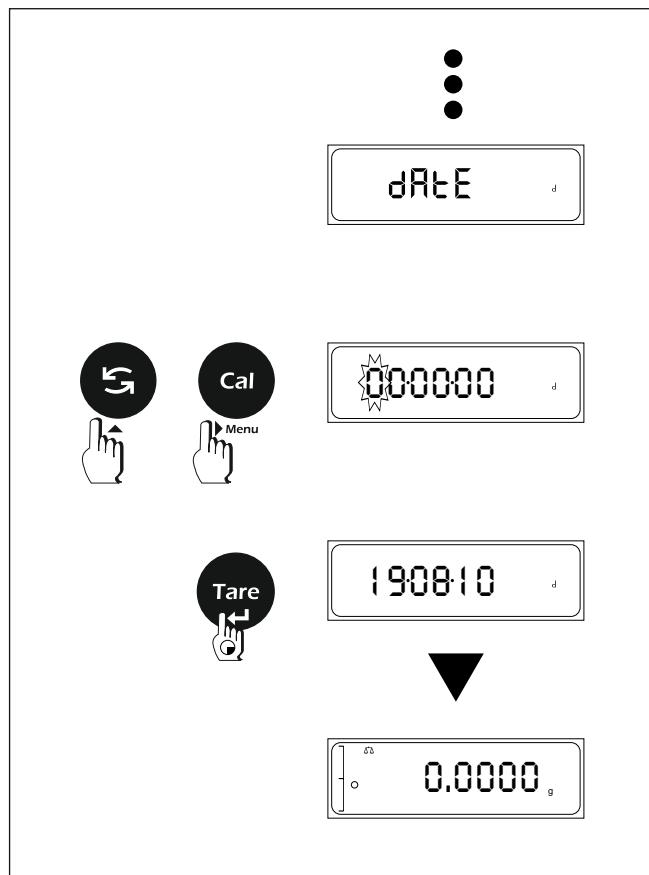

### 7.1.2 SET DATE

- ⇒ Press TARE key, "date" is display
- ⇒ Press TARE key, current date is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press TOGGLE key (▲) to change the value of the Flashing digit.
- ⇒ Press CAL key (►) to shift the flashing digit from Left to Right
- ⇒ After proper setting of date in day, month & year respectively for zeroes starting from left,
- ⇒ Press TARE key to set the date

## 7.2 BATCH ID / SAMPLE ID / TEXT3 DATA Setting

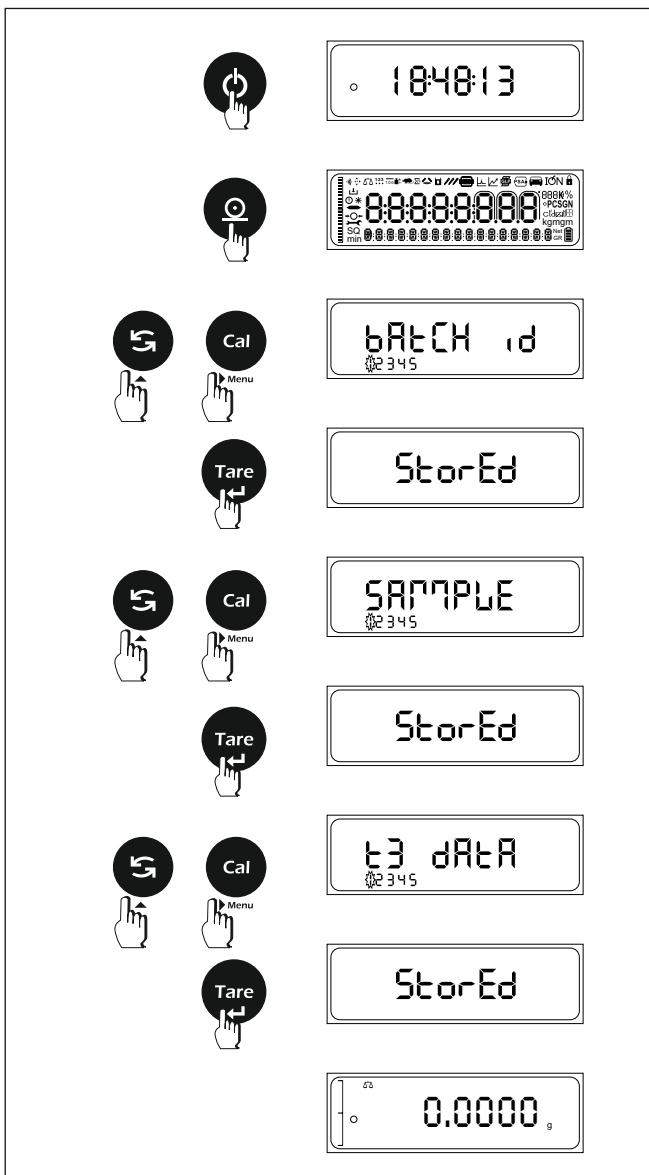

In this menu user can set the Batch identification number & Sample Identification number.

### Operating Instructions

- Press the PRINT key briefly when coming out from stand by or Power on mode.

#### 7.2.1 SET BATCH ID

- Last stored BATCH ID is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- Press TOGGLE key (▲) to change the value of the Flashing digit.
- Press CAL key (►) to shift the flashing digit from Left to Right
- Press the TARE key to store Batch ID Value
- When user has set BATCH ID Value as blank then it will not print the entire BATCH ID line.


#### 7.2.2 SET SAMPLE ID

- Last stored SAMPLE ID is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- Press TOGGLE key (▲) to change the value of the Flashing digit.
- Press CAL key (►) to shift the flashing digit from Left to Right
- Press the TARE key to store SAMPLE ID Value
- When user has set SAMPLE ID Value as blank then it will not print the entire SAMPLE ID line.

#### 7.2.3 SET TEXT3 DATA

- Last stored TEXT3 DATA is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- Press TOGGLE key (▲) to change the value of the Flashing digit.
- Press CAL key (►) to shift the flashing digit from Left to Right
- Press the TARE key to store TEXT3 DATA Value
- When user has set TEXT3 DATA Value as blank then it will not print the entire TEXT3 DATA line.

## 7.3 CUSTOMIZE PRINT SETTING

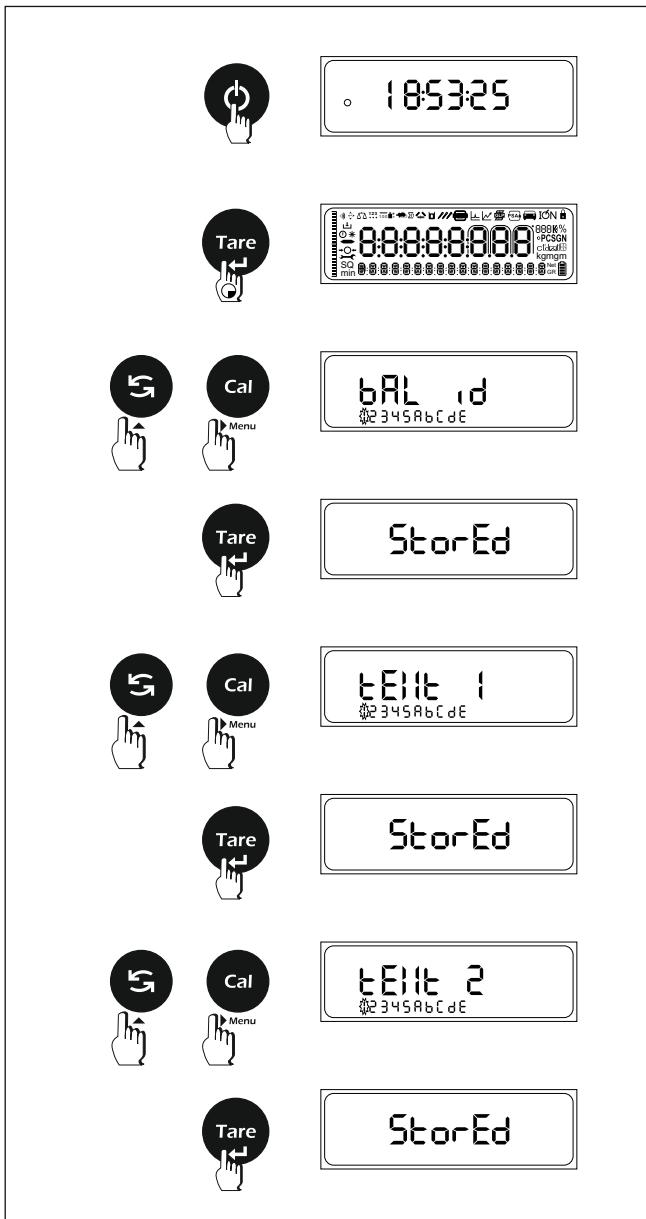

In this menu user can set the Batch ID, Text1, Text2, Text3, Date (On/Off) and Sign (On/Off).

### Operating Instructions

- ⇒ Press the Tare Key for 2 second when coming out from stand by or Power on mode.

#### 7.3.1 SET BALANCE ID


- ⇒ Last stored BALANCE ID is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press TOGGLE key (▲) to change the value of the Flashing digit.
- ⇒ Press CAL key (►) to shift the flashing digit from Left to Right
- ⇒ Press the TARE key to store BALANCE ID Value
- ⇒ When user has set BALANCE ID Value as blank then it will not print the entire BALANCE ID line.

#### 7.3.2 SET TEXT 1

- ⇒ Last stored TEXT1 Value is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press TOGGLE key (▲) to change the value of the Flashing digit.
- ⇒ Press CAL key (►) to shift the flashing digit from Left to Right
- ⇒ Press the TARE key to store TEXT1 Value
- ⇒ When user has set TEXT1 Value as blank then it will not print the entire TEXT1 line.

#### 7.3.3 SET TEXT 2

- ⇒ Last stored TEXT2 Value is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press TOGGLE key (▲) to change the value of the Flashing digit.
- ⇒ Press CAL key (►) to shift the flashing digit from Left to Right
- ⇒ Press the TARE key to store TEXT2 Value
- ⇒ When user has set TEXT2 Value as blank then it will not print the entire TEXT2 line.

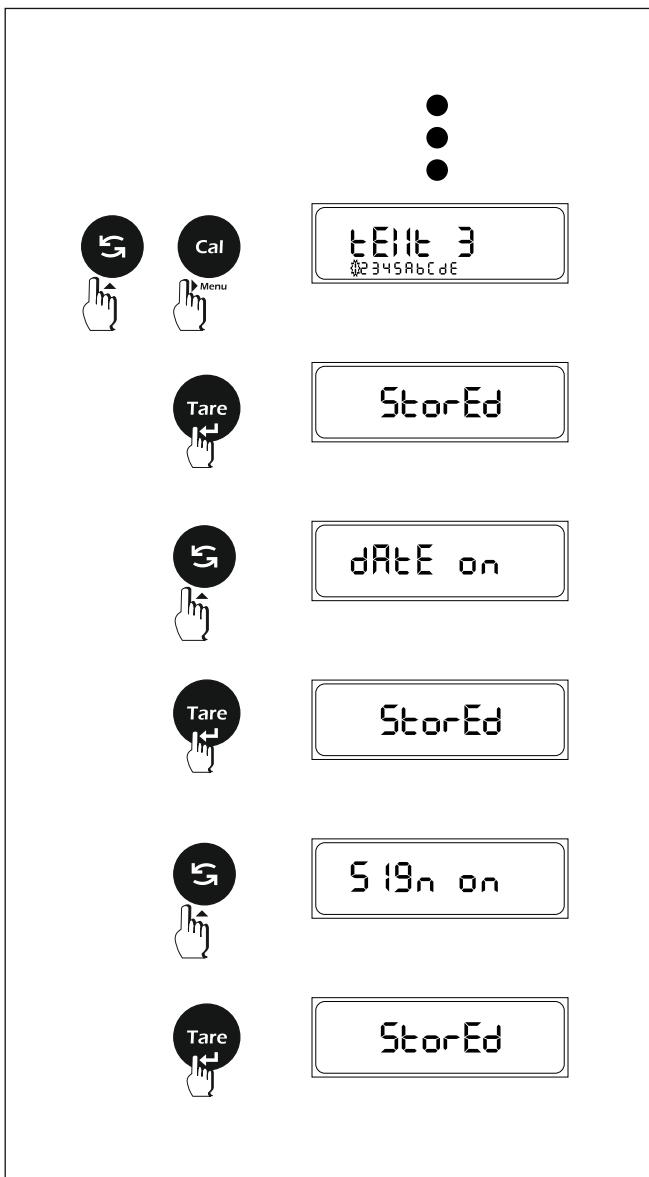

#### 7.3.4 SET TEXT 3

- ⇒ Last stored TEXT3 Value is displayed with first digit flashing. Flashing digit indicates that digit value or place can be changed.
- ⇒ Press TOGGLE key ( ▲ ) to change the value of the Flashing digit.
- ⇒ Press CAL key ( ► ) to shift the flashing digit from Left to Right
- ⇒ Press the TARE key to store TEXT3 Value
- ⇒ When user has set TEXT3 Value as blank then it will not print the entire TEXT3 line.


#### 7.3.5 SET DATE ( ON / OFF )

- ⇒ Last stored DATE value is displayed with "On/Off". On/Off indicate that DATE will be Printed or not.
- ⇒ Press TOGGLE key ( ▲ ) to change the value of "On/Off".
- ⇒ Press TARE key to store DATE (On/Off) Value.

#### 7.3.6 SET SIGN ( ON / OFF )

- ⇒ Last stored SIGN value is displayed with "On/Off". On/Off indicate that SIGN will be Printed or not.
- ⇒ Press TOGGLE key ( ▲ ) to change the value of "On/Off".
- ⇒ Press TARE key to store SIGN (On/Off) Value.

## 7.4 Auto Calibration

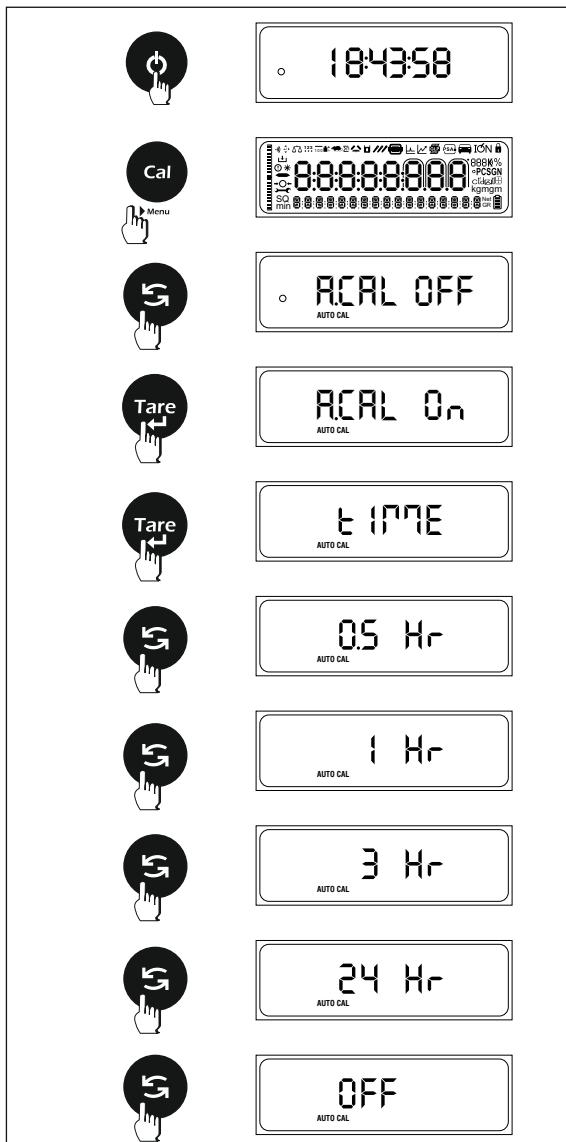

- ⇒ Auto Internal Calibration can be triggered automatically, by the following
  - Time
  - Temperature
  - Power on Calibration

### Operating Instruction

- ⇒ Press the CAL key briefly when coming out from stand by or Power on mode.

#### 7.4.1 Auto CAL Time Settings

Select Auto CAL ON and press the <TARE> key, now press the <TARE> key when the Displays shows TIME to enter time settings.

User can set time value = 0.5 hrs.

User can set time value = 1 hrs.

User can set time value = 2 hrs.


User can set time value = 3 hrs.

User can set time value = 24 hrs.

User can set time value = OFF

Auto Cal triggered due to time will take place irrespective of cal test on or OFF

**Note :** The Above setting is available with balances with internal calibration.

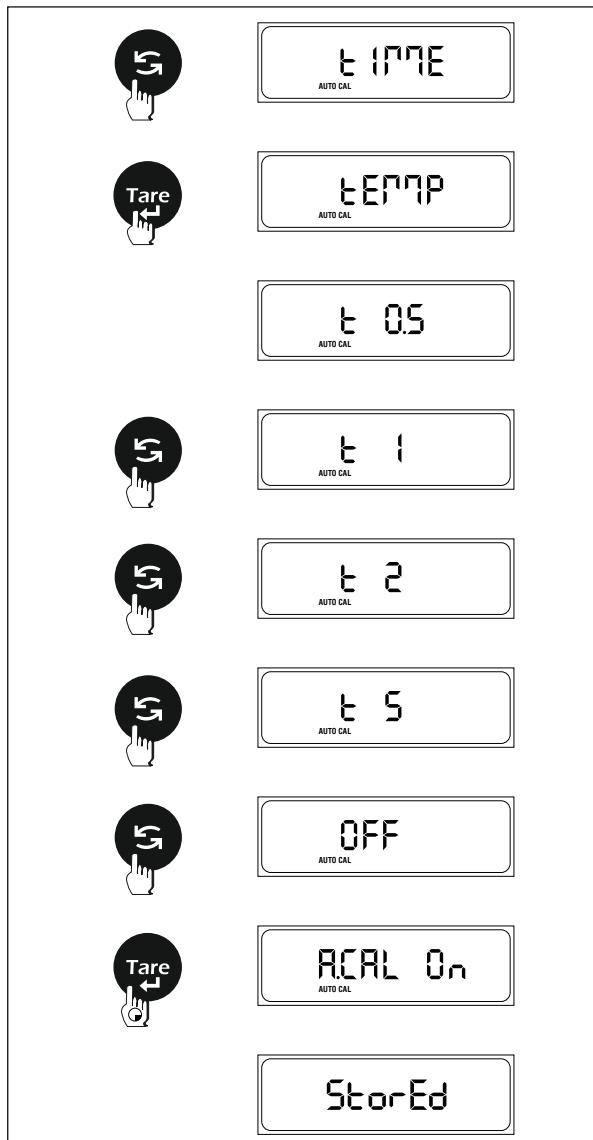

#### 7.4.2 Auto CAL Temperature Settings

Select Auto CAL ON and press the <TARE< key, now press the <TOGGLE> key when the LCM displays TIME, press the <TARE> key to enter temperature settings.

User can set temp. value = 0.5°C.

User can set temp. value = 1°C.


User can set temp. value = 2°C.

User can set temp. value = 5°C.

User can set temp. value = OFF

Auto Cal triggered due to temp. change will take place irrespective of CAL test is On or off

**Note :** The Above setting is available with balances with internal calibration.

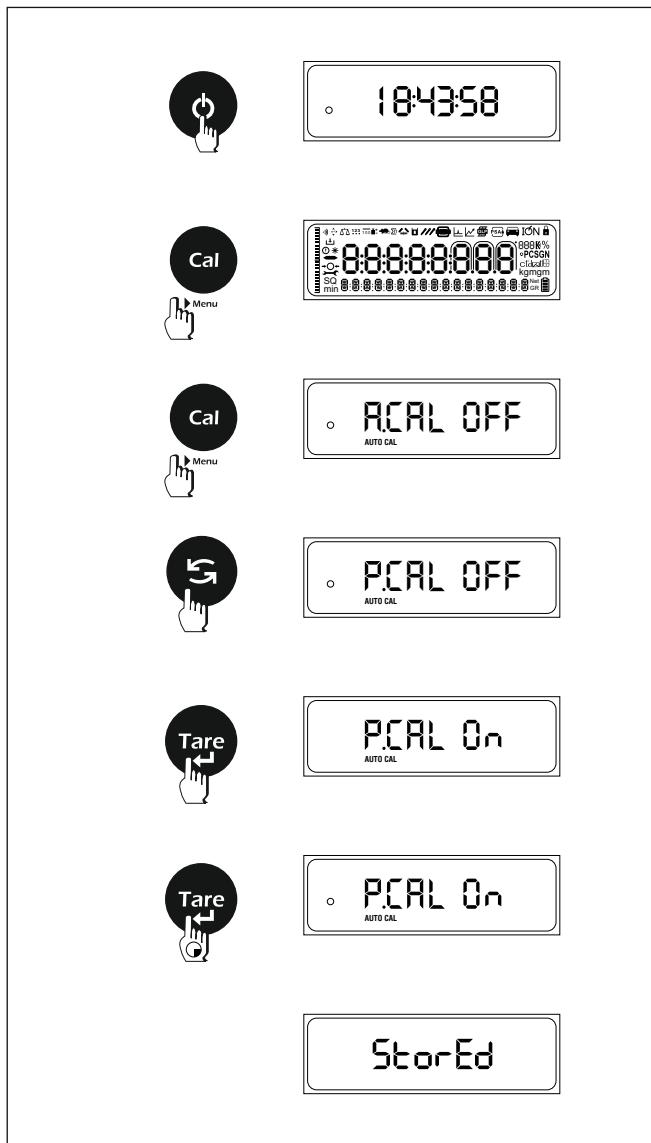

### 7.4.3 Power on Calibration

Press the CAL key when the LCM displays Auto CAL On or Off enter Power ON calibration options.

This setting enables the user to turn on or turn off power on calibration.

Power on calibration will take place every time the balance is powered on.

Power on Cal will take place irrespective of whether CAL Test is On or Off.

**Note :** The Above setting is available with balances with internal calibration.

## 7.5 Windows Direct Communication

The windows direct communication function enables you to send the data from the balance directly to any windows application program for e.g. Microsoft word, excel etc.

The printer settings in the user menu will be applicable to the windows direct communication also i.e. Data Transfer Mode, Baud rate, Parity, Stop Bit and GLP


The settings attributed to windows direct communication are


- Unit ON or OFF.
- Separator type ENTER or TAB.

To enable windows direct communication, make sure that you have turned it on from the windows side as well.

- ⇒ Enter control panel.
- ⇒ Open ACCESSIBILITY OPTIONS from control panel.
- ⇒ In the general tab turn on serial key option.
- ⇒ Set the baud rate and COM port from the settings option.

- ⇒ Click OK to accept the settings for serial key.
- ⇒ Click APPLY and then OK to save the Accessibility options.

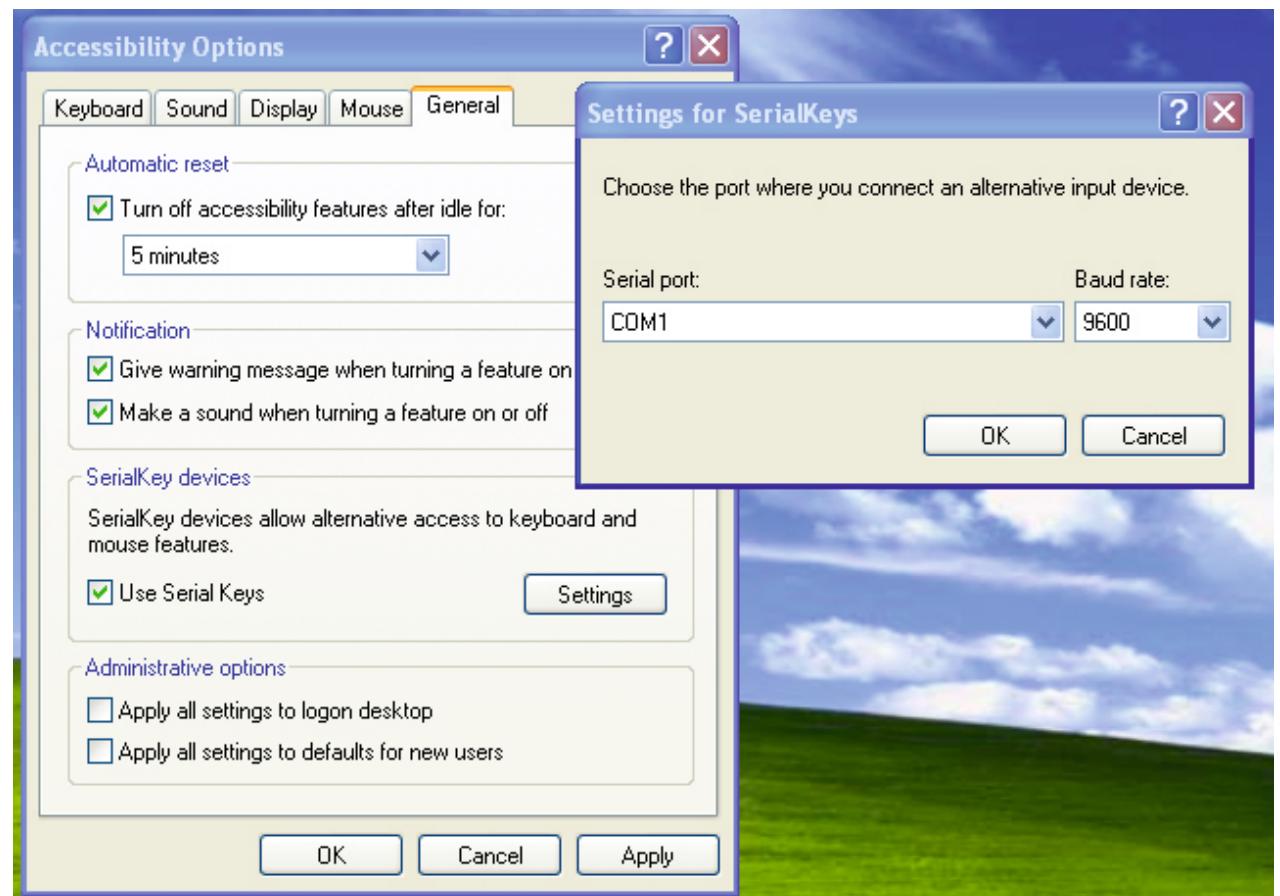

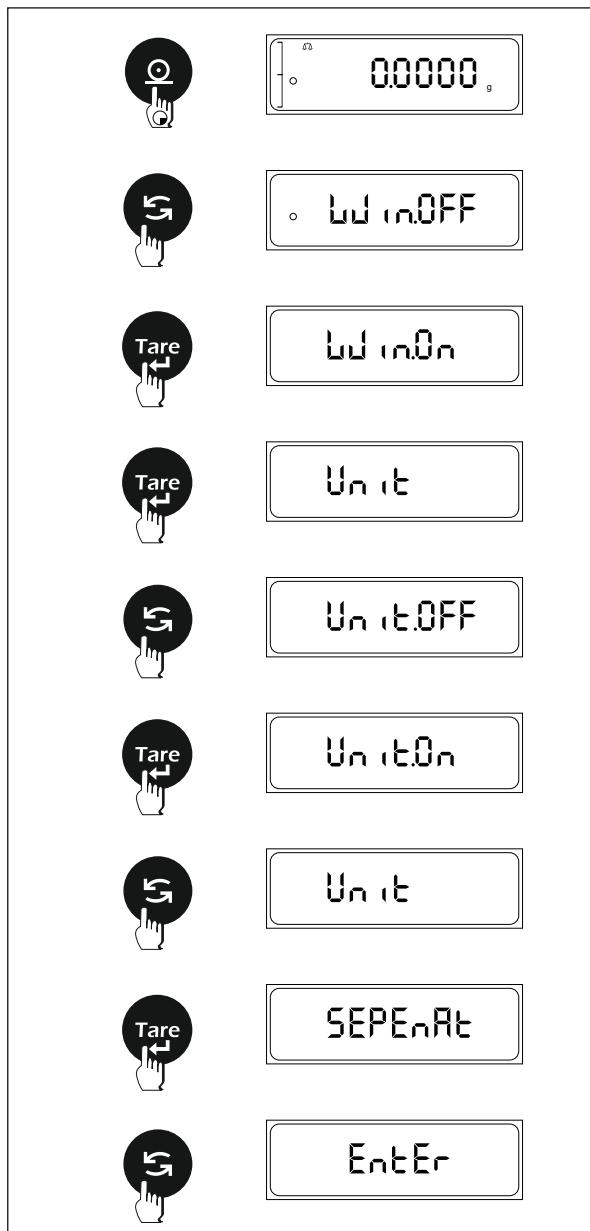

### Windows direct communication settings (Balance Side)


- ⇒ Press and hold the <PRINT> key in simple weighing mode until the windows print menu is prompted.
- ⇒ Press the <TOGGLE> key briefly to change the windows option to ON or OFF. The default option is OFF.

### Windows Unit settings

Select Windows print option as ON and press the <TARE> key, now press the <TARE> key when the LCM displays UNIT to enter unit settings.

User can set Unit option as ON (Along with the numerical value the unit will also be sent to windows).

User can set Unit option as OFF (Only the numerical value will be sent to windows and not the unit).

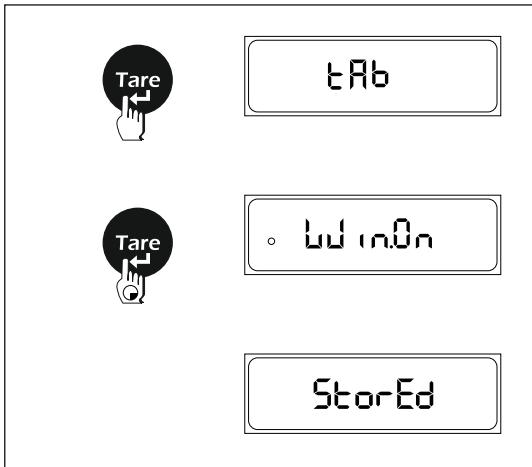

### Windows Separator settings

Select Windows print option as ON and press the <TARE> key, now press the <TARE> key when the LCM displays 'Separat' to enter Separator settings.

User can set SEPERATOR option as ENTER (After every value printed on the windows side an ENTER command is given so every subsequent data will print on new line, in Excel every new data will be printed in new row).

User can set SEPERATOR option as TAB (After every value printed on the windows side a TAB command is given so every subsequent data will printed with tab, in Excel every new data will be printed in new column).

## 8. ISO/GLP-compliant Printout/Record

### Features

You can have the parameters pertaining to the ambient weighing conditions printed before (GLP header) and after (GLP footer) the values of a weighing series. These parameters include:

#### GLP Header :

- Dash Line
- Date
- Time ( Beginning of Measurement )
- Balance Manufacturer
- Balance Model
- Balance Serial Number
- Balance Version Number
- Balance Identification Number of the current sampling operation
- Dash Line
- Text3 ( Editable )
- Batch ID
- Sample ID

#### GLP Footer :

- Dash Line
- Date
- Time ( End of Measurement )
- Field for operator Signature
- Dash Line

The record is output to a ACZET data printer or a computer.

### Settings

Set print option to request & P.tyP GLP

### Function Keys

Press the Print key to output header and first measured value.

End an Application:

Output GLP Footer : Press Cancel Key

End an application program Press Cancel key

## The ISO/GLP-compliant record can contain the following lines:

|                    |             |   |
|--------------------|-------------|---|
| -----              |             | - Dash Line   |
| 05-Oct-23          | 10:35AM     | - Date / Time ( Beginning of Measurement )                        |
|                    | ACZET       | - Balance Manufacturer  |
| <i>Model</i>       | CY224C      | - Balance Model   |
| <i>Ser.No.</i>     | 12345678    | - Balance Serial Number   |
| <i>Ver.No.</i>     | r.1.1.6.5   | - Balance Version Number  |
| <i>Bal. ID.</i>    | S/123       | - Balance Identification Number of the current sampling operation |
| -----              |             | - Dash Line   |
| <i>Product:</i>    | XYZ         | - Text3 ( Editable )  |
| <i>Batch ID:</i>   | T123        | - Batch ID  |
| <i>Sample ID:</i>  | L001        | - Sample ID   |
| <i>nRef</i>        | 10 pcs      | - Counting : Reference Sample Quantity                            |
| <i>wRef</i>        | 5.0052 g    | - Counting : Reference Weight                                     |
| <i>Qnt +</i>       | 14 pcs      | - Counting Result   |
| +                  | 50.0650 g   | - Weighing Result   |
| +                  | 250.3250 ct | - Weighing Result   |
| -----              |             | - Dash Line   |
| 05-Oct-23          | 10:35AM     | - Date / Time ( End of Measurement )                              |
| <i>Signature :</i> | .....       | - Field for operator Signature                                    |
| -----              |             | - Dash Line   |

## The ISO/GLP-compliant record can contain the following lines:

|                          |           |   |
|--------------------------|-----------|---|
| -----                    |           | - Dash Line   |
| 05-Oct-23                | 10:35AM   | - Date / Time ( Beginning of Measurement )                        |
|                          | ACZET     | - Balance Manufacturer  |
| <i>Model</i>             | CY224C    | - Balance Model   |
| <i>Ser.No.</i>           | 12345678  | - Balance Serial Number   |
| <i>Ver.No.</i>           | r.1.1.6.5 | - Balance Version Number  |
| <i>Bal. ID.</i>          | S/123     | - Balance Identification Number of the current sampling operation |
| -----                    |           | - Dash Line   |
| <i>Product :</i>         | XYZ       | - Text3 ( Editable )  |
| <i>Batch ID :</i>        | T123      | - Batch ID  |
| <i>Sample ID :</i>       | L001      | - Sample ID   |
| <i>Calibration :</i>     | External  | - Calibration / Adjustment Mode                                   |
| <i>W-ID</i>              | -----     | - Weight ID   |
| <i>Temperature</i>       | 32.898' C | - Temperature   |
| <i>Set +</i>             | 20.00 g   | - Calibration Weight  |
| <i>Diff.</i>             | 0.00 g    | - Diff. After Calibration   |
| <i>External Cal Done</i> |           | - Confirmation of Completed Calibration                           |
| <i>Diff.</i>             | 0.00 g    | - Difference from nominal value after Calibration                 |
| -----                    |           | - Dash Line   |
| 05-Oct-23                | 10:35AM   | - Date / Time ( End of Measurement )                              |
| <i>Signature :</i>       | -----     | - Field for operator Signature                                    |
| -----                    |           | - Dash Line   |

## 9. Data Interface

### Purpose

Your balance is equipped with an interface port for connection to a computer or other peripheral device. You can use an on-line computer to change, start and/or monitor the functions of the balance and the application programs.

### Features

- Type of interface: Serial interface
- Operating mode: Full duplex
- Standard: RS-232
- Transmission rates: 300; 600; 1,200; 2,400; 4,800; 9,600; 19,200 baud 57600
- Parity: Mark, space, odd, even, none
- Character format: 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits
- Handshake: None
- Data output format of the balance : 26 characters

### Factory settings:

Transmission rate: 1,200 baud (9600)

Parity: Odd (none)

Stop bits: 1 stop bit

Handshake: None

Print manually/automatically: Manual at stability

### Preparation

- See "Pin Assignments"

## 9.1 Output Format with 26 Characters

The following characters can be output, depending on the characters displayed on the balance :

Normal Operation

| Position | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | 15 | 16 | 17 | 18 | 19 | 20 | 21 | 22 | 23 | 24 | 25 | 26 |
|----------|---|---|---|---|---|---|---|---|---|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|
|          | * | * | * | * | * | + | D | D | D | D  | D  | D  | D  | D  | D  | D  | D  | D  | D  | *  | U  | U  | U  | U  | LF | CR |
| or       | * | * | * | * | * | - | D | D | D | D  | D  | D  | D  | D  | D  | D  | D  | D  | D  | *  | U  | U  | U  | U  | LF | CR |
| or       | I | I | I | * | + | D | D | D | D | D  | D  | D  | D  | D  | D  | D  | D  | D  | D  | *  | U  | U  | U  | U  | LF | CR |

\* : Space

D : Digit or letter

U : Unit Symbol

CR : Carriage Return

LF : Line Feed

I : ID code Character

Special Codes

| Position | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | 15 | 16 | 17 | 18 | 19 | 20 | 21 | 22 | 23 | 24 | 25 | 26 |
|----------|---|---|---|---|---|---|---|---|---|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|
|          | - | - | - | - | - | - | - | - | - | O  | L  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | LF | CR |    |
| or       | - | - | - | - | - | - | - | - | - | U  | L  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | LF | CR |
| or       | - | - | - | - | - | - | - | - | - | O  | r  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | LF | CR |
|          | - | - | - | - | - | - | - | - | - | L  | L  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | LF | CR |
|          | - | - | - | - | - | - | - | - | - | H  | H  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | -  | LF | CR |

OL : Space

Or : Digit or letter

HH : Unit Symbol

UL : Carriage Return

LL : Line Feed

## Data Output Examples + 123.4567 g

| Position | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | 15 | 16 | 17 | 18 | 19 | 20 | 21 | 22 | 23 | 24 | 25 | 26 |
|----------|---|---|---|---|---|---|---|---|---|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|----|
|          |   |   |   |   |   |   |   | + |   |    |    |    |    | 1  | 2  | 3  | .  | 4  | 5  | 6  | 7  |    | g  | LF | CR |    |
| or       |   |   |   |   |   |   |   |   |   |    |    |    |    | 6  | 1  | 7  | .  | 2  | 8  | 3  | 5  |    | c  | t  | LF | CR |
| or       | N | 1 |   |   |   |   |   |   |   |    |    |    |    | 2  | 0  | .  | 0  | 0  | 0  | 0  | 0  |    | g  | LF | CR |    |
| or       | T | o | t |   |   |   |   | + |   |    |    |    |    | 6  | 0  | .  | 0  | 0  | 0  | 0  | 0  |    | g  | LF | CR |    |

|                  |   |  |
|------------------|---|--|
| Position 1 - 4   | : | ID code Character or Space                       |
| Position 5       | : | Sign   |
| Position 6 - 20  | : | Weight with Decimal Point; leading zeros = space |
| Position 21      | : | Space  |
| Position 22 - 24 | : | Unit Symbol or Space                             |
| Position 25      | : | Line Feed  |
| Position 26      | : | Carriage Return                                  |

### ID code

| characters  | Meaning   |
|-------------|---|
| <b>nRef</b> | Counting: Reference sample quantity                       |
| <b>wRef</b> | Piece Counting, Percentage Weighing :<br>Reference weight |
| <b>Qnt</b>  | Piece Counting: Quantity                                  |
| <b>pRef</b> | Weighing in percent: Reference percentage                 |
| <b>Pct</b>  | Weighing in percent: Reference percentage                 |
| <b>Cnt</b>  | Animal weighing: No. of sub-weighing operations           |
| <b>xNt</b>  | Animal weighing: Calculated average                       |

### ID Code

| Characters | Meaning   |
|------------|---|
| <b>N1</b>  | Formulation, Totalization Net : N1                |
| <b>N</b>   | Formulation, Totalization Net N                   |
| <b>Tot</b> | Formulation, Totalization : Total Weight          |
| <b>Pur</b> | density : Purity of Gold                          |
| <b>Den</b> | Density : density of sample                       |
| <b>Pip</b> | Pipette Calibration                               |
| <b>Sta</b> | Statistics : to obtain the statistics of the data |

## 9.2 Data Input Format

You can connect a computer to your balance to send commands via the balance interface port to control balance functions and applications.

Format for commands

|   |              |      |   |
|---|--------------|------|---|
| [ | Command Code | Data | ] |
|---|--------------|------|---|

- [: it shows start of command frame.
- Command Code: it shows which functionality to be carried out for this command frame.
- Data: This field in frame is optional and it is intended to provide data information between Bi-directional communications.
- ]: it shows end of command frame.


Commands

[W] : If host computer send this command to balance then balance will Send weight with current unit.

[T] : If host computer send this command then balance will do taring in balance. If stability is not achieved within 45 second then it comes to that specific feature till that time it shows “-----” on LCM.

## 9.3 Cabling Diagram

- For connecting a computer or other peripheral device to the balance using the RS-232 protocol and cables up to 15m (50 ft.) long.

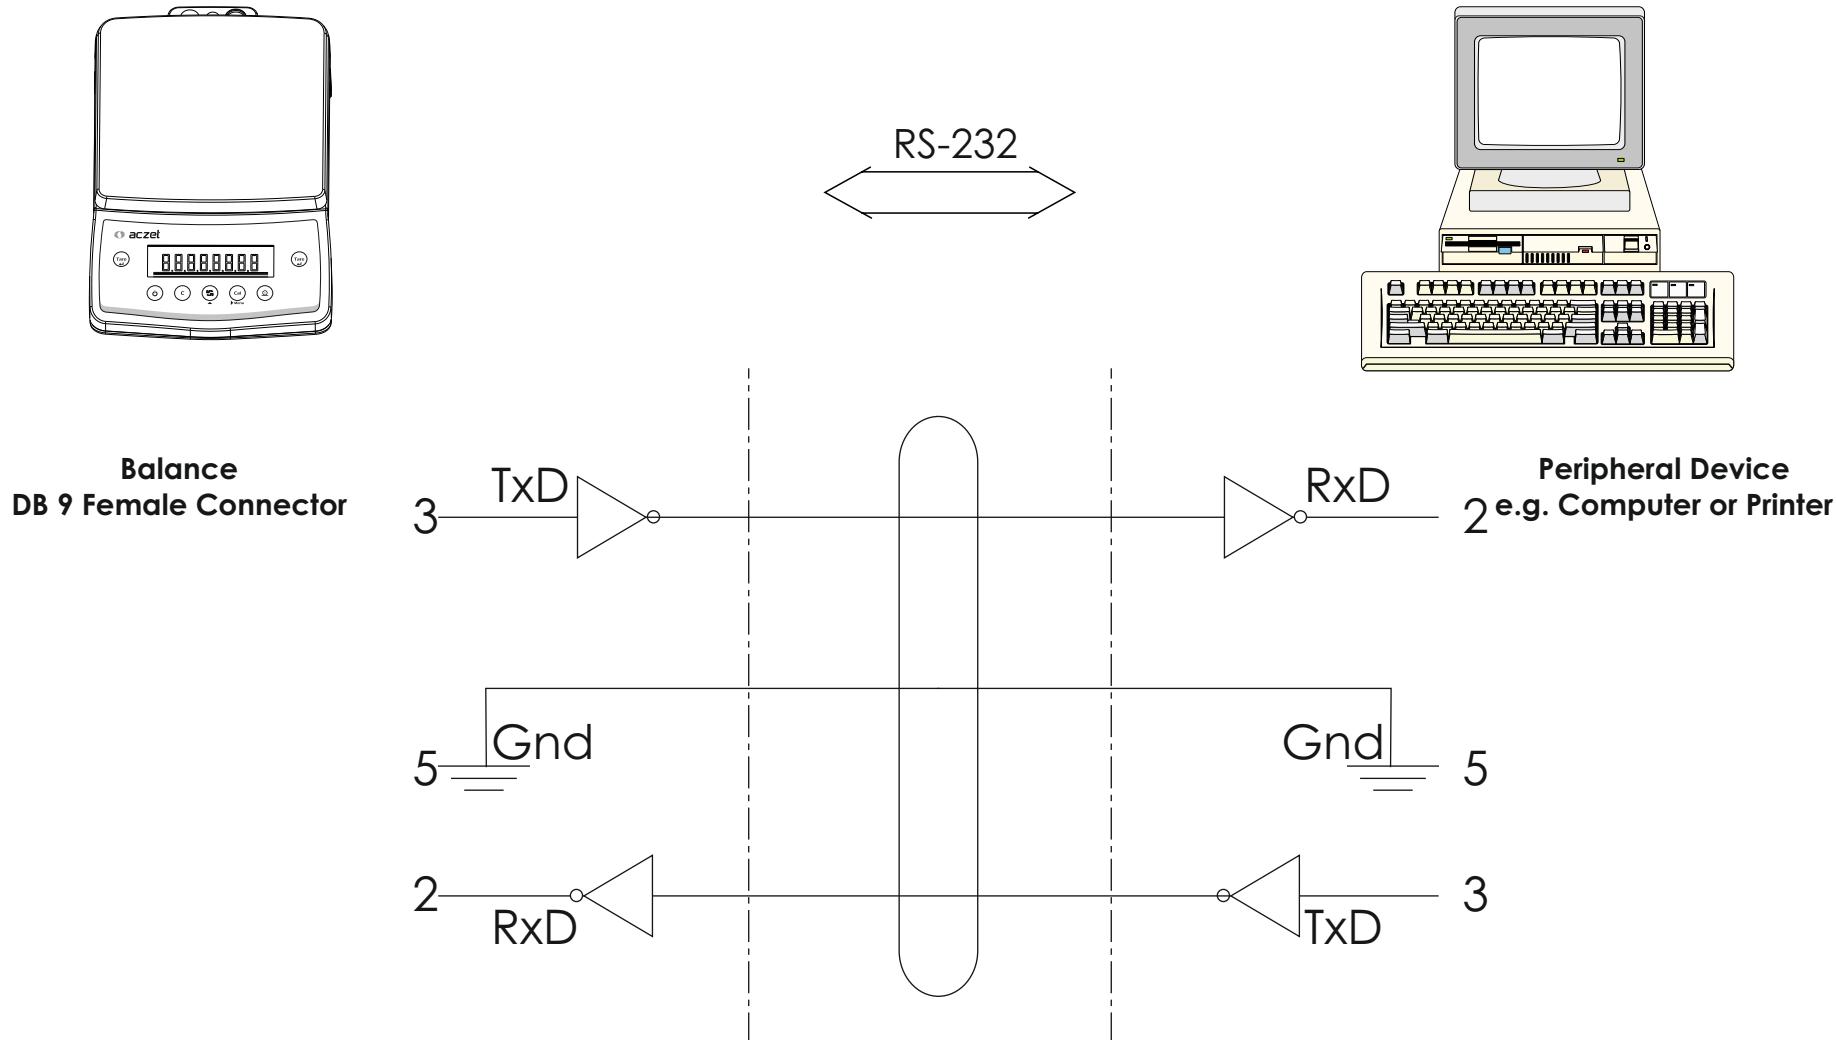

## 10. Error Codes

| Display | Cause  | Solution   |
|---------|--|--|
| --OL--  | Overload   | Remove excess weight from the weighing pan.  |
| --UL--  | Under load   | <ul style="list-style-type: none"> <li>Keep weighing Pan on Weighing Shaft.</li> <li>Check whether weighing pan is positioned properly.</li> </ul>                         |
| Error 1 | Weight set is to low for storing any reference at PCS, %, Custom Unit or Check Weighing.   | Increase weight on the pan.  |
| Error 2 | While calibrating the scale, the load on the pan is more than 10% of the capacity. (During power on of the scale.)   | Switch OFF the Balance and Switch ON again without any load on the pan.  |
| Error 3 | <p>Calibration</p> <ul style="list-style-type: none"> <li>User does not keep any weight on the pan within 60 second.</li> <li>Weight load on the pan is not within the tolerance limit.</li> </ul> | <ul style="list-style-type: none"> <li>Add the calibration weight on the pan when demanded by the balance</li> <li>Calibrate with the exact Calibration Weight.</li> </ul> |
| Error 4 | GLP is ON and user tries to enter in to the User Menu before the footer is printed.  | Print the footer first, by pressing <CANCEL> key, and then access the USER MENU.   |
| Error 5 | <p>Calibration</p> <p>Display shows any weight other than 0.00 and user tries to Calibrate the balance</p>   | Tare the balance or enter Calibration procedure when "0.00 g" is displayed.  |
| Error 7 | Incorrect value of TIME or DATE.   | Enter proper value of TIME or DATE.  |

| Display                               | Cause  | Solution   |
|---------------------------------------|--|--|
| Error 8                               | Last stored PRINT option is AUTO or AUTO LOAD or CONTINUOUS and user tries to set GLP ON from USER MENU.     | Change the print option to Print on REQUEST and then turn GLP ON.            |
| Error 9                               | RTC not operational.   | Contact Aczet Service center.  |
| Error 29                              | Error 2 Calibration Error + RTC Error.   | Contact Aczet Service center.  |
| Error 39                              | Error 3 Calibration Error + RTC Error.   | Contact Aczet Service center.  |
| The weight readout changes constantly | Unstable ambient conditions<br>A foreign object is caught between the load plate and the balance/scale frame | Set up the balance/scale in another area Remove the foreign object           |
| The weight readout is obviously wrong | The balance has not been calibrated / adjusted.<br>The balance was not zeroed before weighing.               | Calibrate / Adjust the balance.<br>Tare or Zero the balance before weighing. |

# 11. Care & Maintenance

## Service

Regular servicing by a ACZET technician will extend the service life of your balance and ensure its continued weighing accuracy. ACZET can offer you service contracts, with your choice of regular maintenance intervals.

The optimum maintenance interval depends on the operating conditions at the place of installation and on the individual tolerance requirements.

## Repairs

Repair work must be performed by trained service technicians. Any attempt by untrained persons to perform repairs may lead to hazards for the user.

## Cleaning

- Unplug the DC adapter from the wall outlet (mains supply). If you have an interface cable connected to the balance/scale port, unplug it from the port.
- Make sure that no liquid enters the balance/scale housing
- Do not use any aggressive cleaning agents (solvents or similar agents)
- Clean the balance/scale using a piece of cloth which has been wet with a mild detergent (soap)
- After cleaning, wipe down the balance/scale with a soft, dry cloth

## **Cleaning Stainless Steel Surfaces**

- Clean all stainless steel parts regularly. Remove the stainless steel weighing pan and thoroughly clean it separately. Use a damp cloth or sponge to clean any stainless steel parts on the scale. You can use any commercially available household cleaning agent that is suitable for use on stainless steel. Clean stainless steel surfaces by wiping them down. Then clean the weighing pan thoroughly, making sure to remove all residues. Use a damp cloth or sponge to wipe down any stainless steel parts on the scale again. Afterwards, allow the scale to dry. If desired, you can apply oil to the cleaned surfaces as additional protection.
- Do not use stainless steel cleaning agents that contain soda lye (caustic), acetic acid, hydrochloric acid, sulfuric acid or citric acid. The use of scrubbing sponges made of steel wool is not permitted. Solvents are permitted for use only on stainless steel parts.

## **Safety Inspection**

If there is any indication that safe operation of the balance/scale with the DC adapter is no longer warranted:

- Turn off the power and disconnect the equipment from DC power immediately
- Lock the equipment in a secure place to ensure that it cannot be used for the time being.
- Safe operation of the balance/scale with the DC adapter is no longer ensured when:
  - There is visible damage to the DC adapter.
  - The DC adapter no longer functions properly.
  - The DC adapter has been stored for a relatively long period under unfavorable conditions.

## **LIMITED WARRANTY**

ACZET products are warranted against defects in materials and workmanship from the date of delivery through the duration of the warranty period. During the warranty period Aczet will repair, or, at its option, replace any component (s) that proves to be defective at no charge, provided that the product is returned, freight prepaid, to ACZET.

This warranty does not apply if the product has been damaged by accident or misuse, exposed to radioactive or corrosive materials, has foreign material penetrating to the inside of the product, or as a result of service or modification by other than ACZET. In lieu of a properly returned warranty registration card, the warranty period shall begin on the date of shipment to the authorized dealer. No other express or implied warranty is given by Aczet Pvt. Ltd.

As warranty legislation differs from state to state and country to country, please contact aczet or your local ACZET dealer for further details.

ACZET service center will repair the product free of charge subject to terms & condition mentioned below.

### **TERMS & CONDITION**

1. It covers only weighing balance purchased from authorized channel and does not cover accessories like Battery, Adaptor, RS232 cable, Pan, Pan support etc
2. It does not cover the product of which model and serial number has been altered, removed or defaced and / or is open by unauthorized person and found void sticker has been tampered.
3. This warranty is non-transferable and applicable only to first end user purchasing the product from authorized dealer.
4. For repair based on this warranty you need to hand over this product or send this product to address mentioned in warranty card in original packing, enclosing copy of this warranty card.'
5. Aczet Pvt. Ltd. shall not be liable for any consequential damages.

# WARRANTY REGISTRATION

## ACZET PVT.LTD.



E2, Plot No. 15, WICEL Estate, Opp. Seepz Gate no. 1,  
Andheri (E), Mumbai - 400 093. Maharashtra, India  
e-mail :- [service@aczet.com](mailto:service@aczet.com) • web.: [www.aczet.com](http://www.aczet.com)  
Tel. No. :- +91-22-4243 7700

NAME :-

ADDRESS :-

TEL NO. :-

SERIAL NO. :-

MODEL NO. :-

PURCHASE DATE :-

WARRANTY PERIOD :-

### BRANCH / DISTRIBUTOR / DEALER CONTACT DETAILS

STAMP / SIGN

Owners Signature / Date

SEND YOUR WARRANTY CARD DULY FILL TO ABOVE EMAIL FOR REGISTRATION


## 12. Dimensional Drawing

### Analytical Balances

(CY(0.1mg)Series

Balances)


Draft Shield High

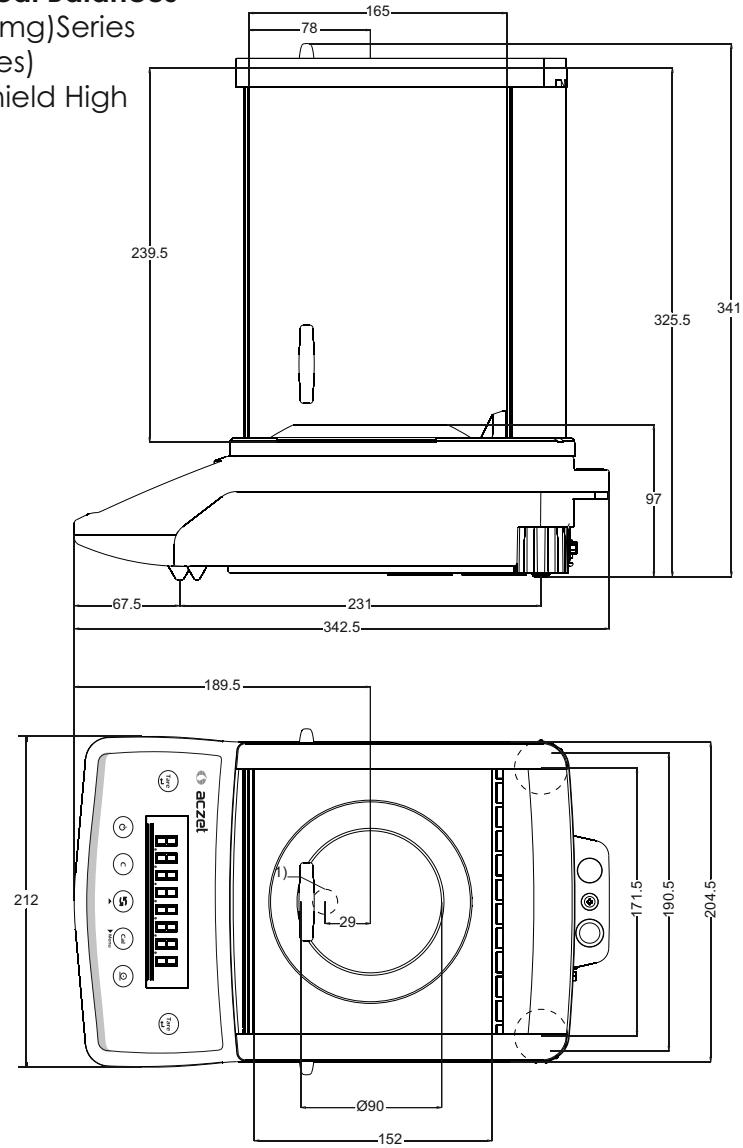


### Carat Balances

(CY(0.001ct) Series Balances)


Draft Shield Low

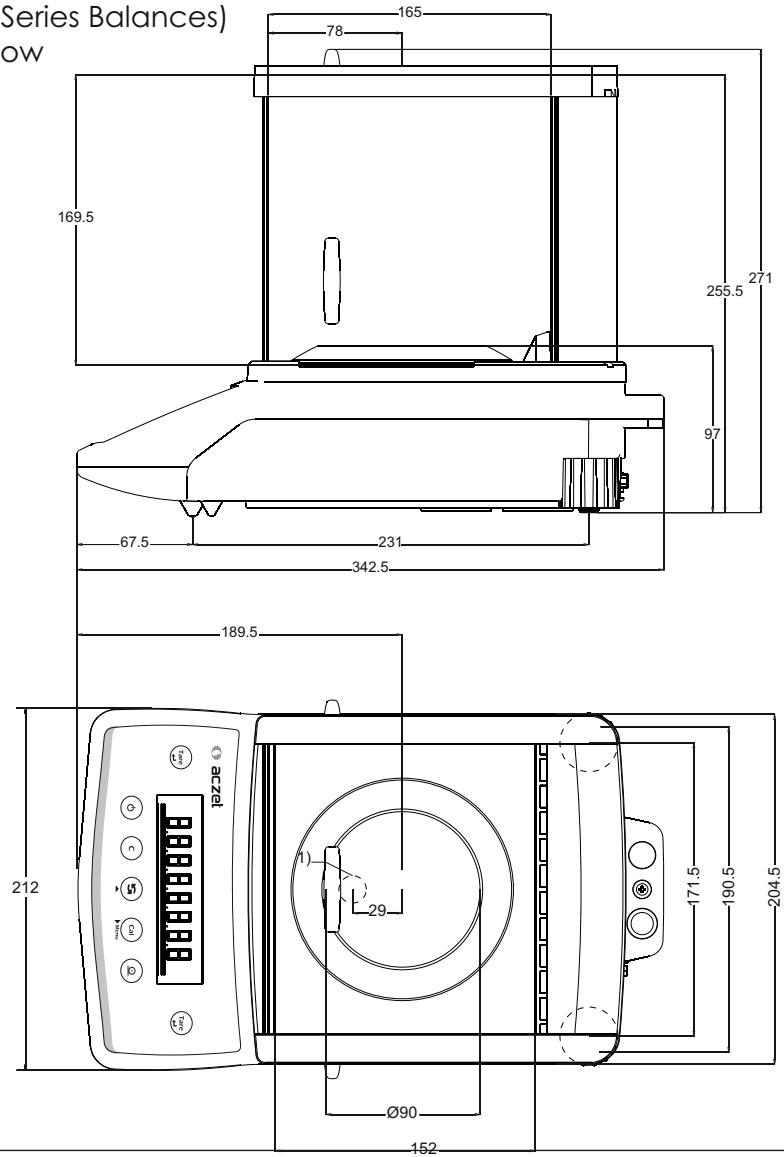


**Top Loading Precision Balances**  
 (CY (10mg) Series Balances)  
 No Draft Shield

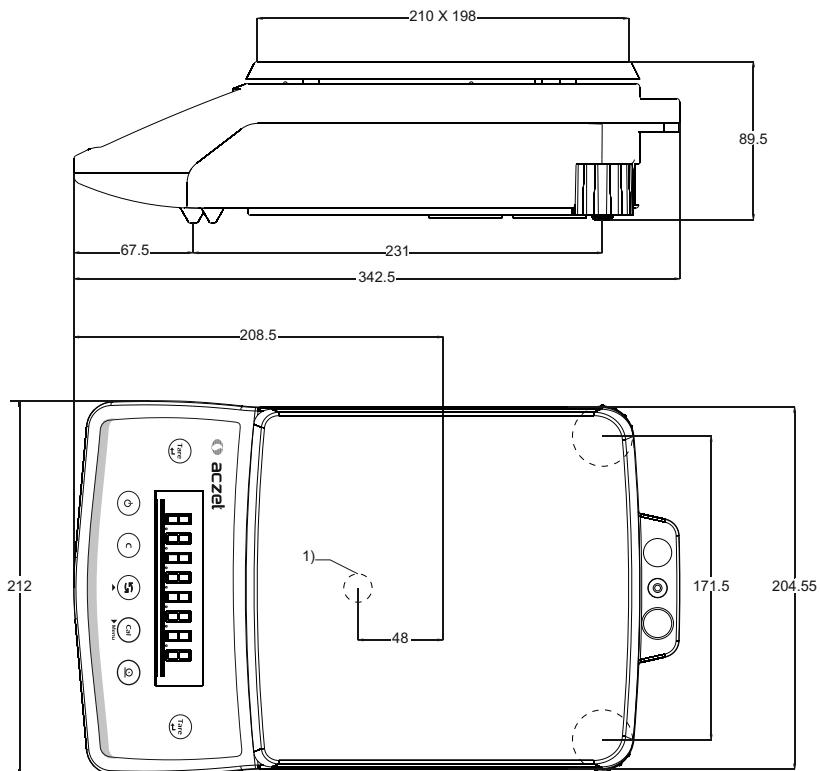

**Precision Balances**  
 (CY (1mg) Series Balances)  
 Draft Shield Low

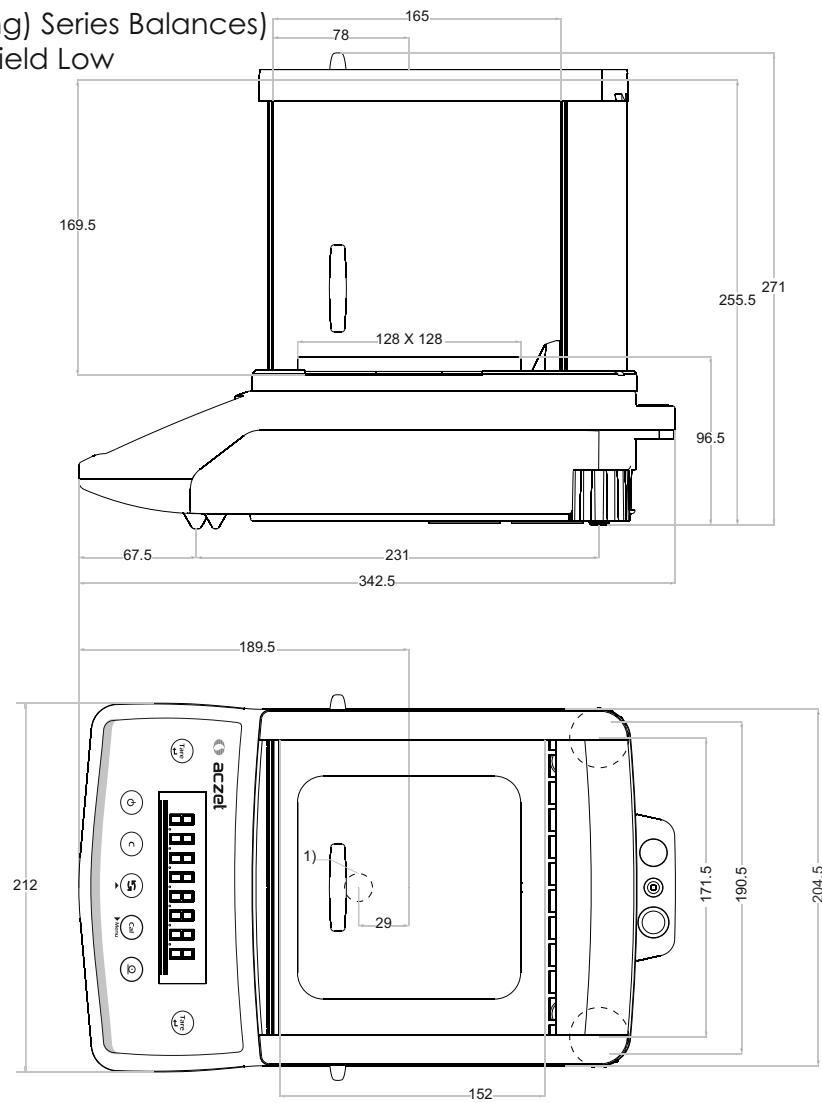


**High Capacity Precision Balances**  
(CY (100mg) Series Balances)

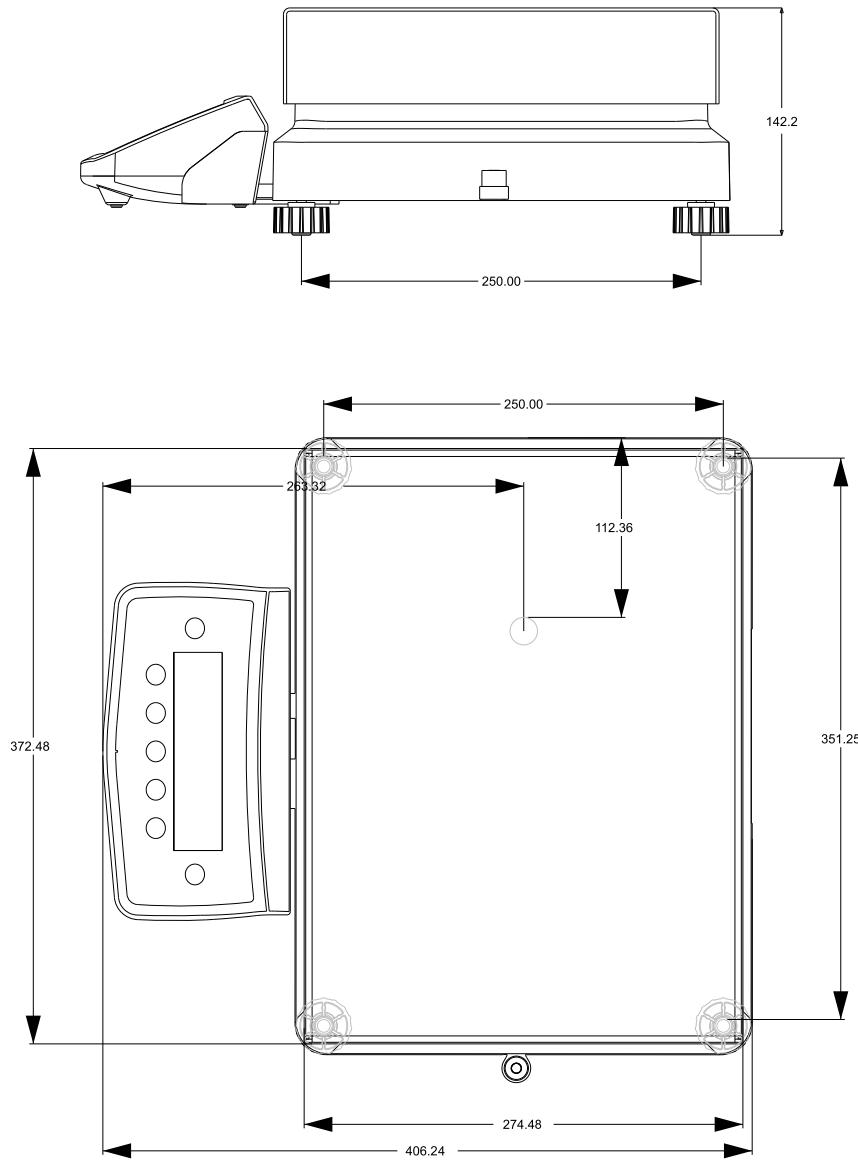

## High Capacity Precision Balances

(CY (1mg) Series Balance with wind shield)

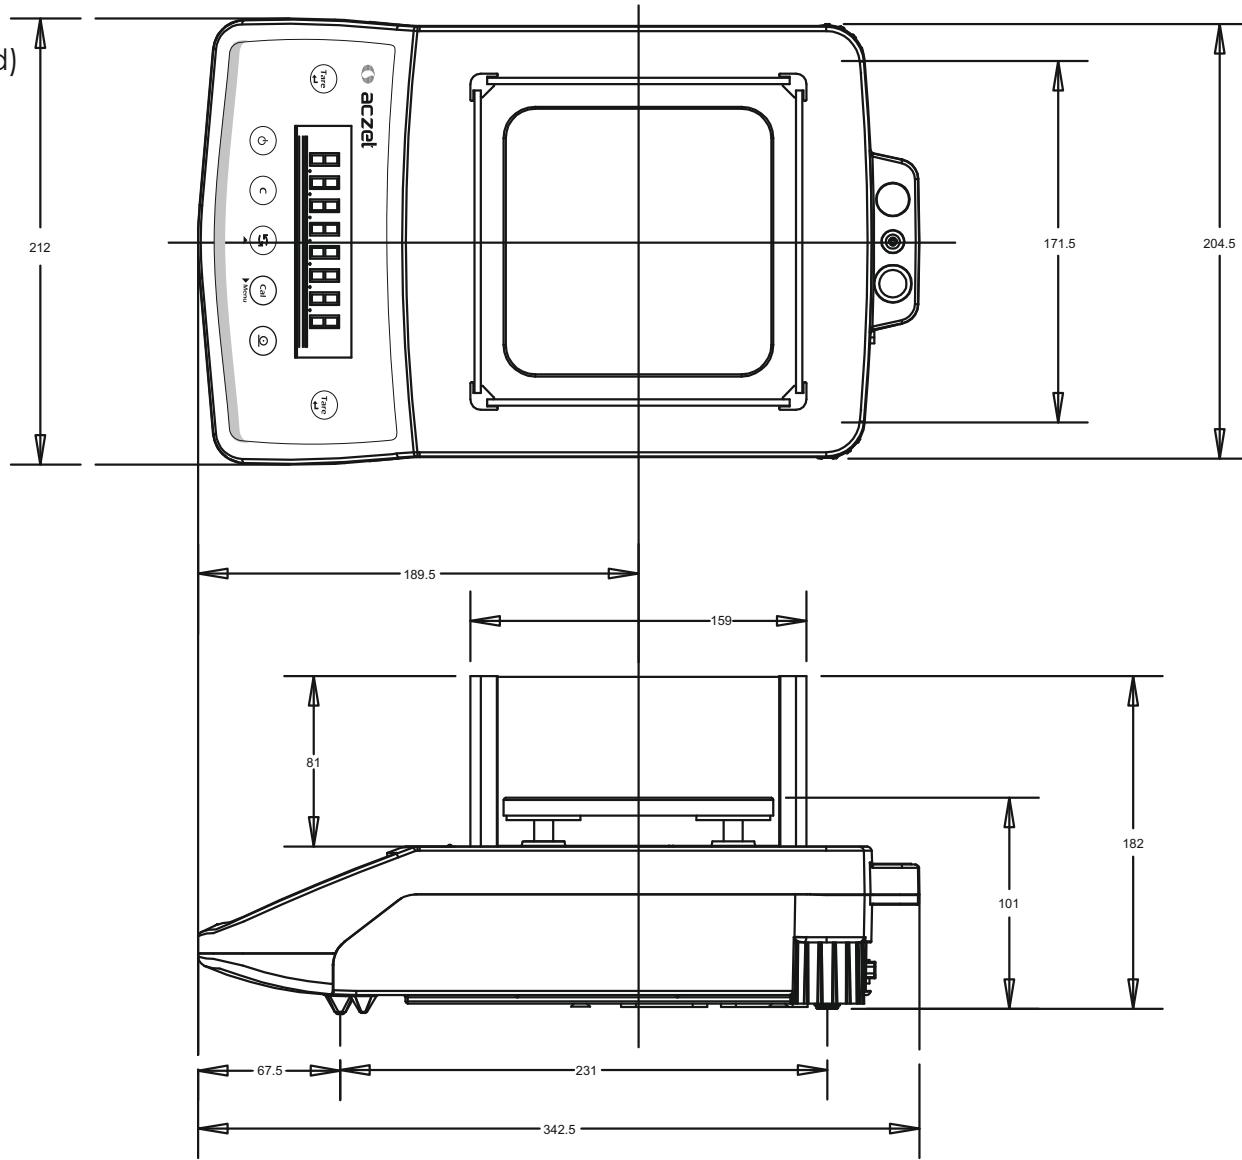

## 13. Specifications

### Analytical Balances

| Model   |      | CY 64C   | CY 124C                | CY 224C     | CY 304C     | CY 324C     | CY 404C     |
|---|------|--|------------------------|-------------|-------------|-------------|-------------|
| Weighing Capacity   | g    | 60   | 120                    | 220         | 301         | 320         | 401         |
| Readability (d)   | mg   | 0.1  | 0.1                    | 0.1         | 0.1         | 0.1         | 0.1         |
| Accuracy (e)  | mg   | 1  | 1                      | 1           | 1           | 1           | 1           |
| Tare Range (Subtractive)                                    | g    | -65  | -120                   | -220        | -301        | -320        | -401        |
| Repeatability (std. deviation)                              | <=mg | 0.1  | 0.1                    | 0.1         | 0.1         | 0.1         | 0.1         |
| Linearity   | <=mg | 0.2  | 0.2                    | 0.2         | 0.3         | 0.3         | 0.3         |
| Weighing Class  |      | I  | I                      | I           | I           | I           | I           |
| Response time (average)                                     | s    | 3 sec.   |                        |             |             |             |             |
| Operating temperature range                                 | °C   | 18° to 30°C  | 18° to 30°C            | 18° to 30°C | 18° to 30°C | 15° to 30°C | 15° to 30°C |
| Calibration   | °C   | Internal   | Internal               | Internal    | Internal    | Internal    | Internal    |
| External calibration weight (of at least accuracy class...) | g    | 25 (E2)  | 50 (E2)                | 100 (E2)    | 200 (E2)    | 25 (E2)     | 10 (E2)     |
| Net Weight, approx.   | kg   | 8kg  |                        |             |             |             |             |
| Pan size  | mm   | 90 Ø   |                        |             |             |             |             |
| Weighing chamber height                                     | mm   | 228.5  |                        |             |             |             |             |
| Dimensions (W x D x H)                                      | mm   | 342.5 x 212 x 341  |                        |             |             |             |             |
| DC power source / Power requirements                        | V~   | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             | ⊕           | ⊖           |
| Frequency   | Hz   | 50 / 60Hz  |                        |             |             |             |             |
| Power consumption (average)                                 | VA   | maximum 18; typical 9  |                        |             |             |             |             |
| Selectable weight units                                     |      | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |             |             |
| Built-in-interface  |      | RS-232/USB   |                        |             |             |             |             |
| Format  |      | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |                        |             |             |             |             |
| Parity  |      | Mark, Space, Odd, even, none   |                        |             |             |             |             |
| Transmission rates :  |      | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |                        |             |             |             |             |
| Handshake mode  |      | None   |                        |             |             |             |             |

## Analytical Balances

| Model   |      | CY 64  | CY 124      | CY 224      | CY 324      | CY 404      |
|---|------|--|-------------|-------------|-------------|-------------|
| Weighing Capacity   | g    | 61   | 120         | 220         | 320         | 401         |
| Readability (d)   | mg   | 0.1  | 0.1         | 0.1         | 0.1         | 0.1         |
| Accuracy (e)  | mg   | 1  | 1           | 1           | 1           | 1           |
| Tare Range (Subtractive)                                    | g    | -61  | -120        | -220        | -320        | -401        |
| Repeatability (std. deviation)                              | <=mg | 0.1  | 0.1         | 0.1         | 0.1         | 0.1         |
| Linearity   | <=mg | 0.2  | 0.2         | 0.2         | 0.3         | 0.3         |
| Weighing Class  |      | I  | I           | I           | I           | I           |
| Response time (average)                                     | s    | 3 sec.   |             |             |             |             |
| Operating temperature range                                 | °C   | 18° to 30°C  | 18° to 30°C | 18° to 30°C | 15° to 30°C | 15° to 30°C |
| Calibration   | °C   | External   | External    | External    | External    | External    |
| External calibration weight (of at least accuracy class...) |      | 25 (E2)  | 50 (E2)     | 100 (E2)    | 25 (E2)     | 10 (E2)     |
| Net Weight, approx.   | g    | 8kg  |             |             |             |             |
| Pan size  | kg   | 90 Ø   |             |             |             |             |
| Weighing chamber height                                     | mm   | 228.5  |             |             |             |             |
| Dimensions (W x D x H)                                      | mm   | 342.5 x 212 x 341  |             |             |             |             |
| DC power source / Power requirements                        | mm   | DC Adapter, input 100 ~ 240 0.8A output 12V / 0.9A   | ⊕           | ⊖           | ⊖           |             |
| Frequency   | V~   | 50 / 60Hz  |             |             |             |             |
| Power consumption (average)                                 | Hz   | maximum 18; typical 9  |             |             |             |             |
| Selectable weight units                                     | VA   | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |             |             |             |             |
| Built-in-interface  |      | RS-232/USB   |             |             |             |             |
| Format  |      | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |             |             |             |             |
| Parity  |      | Mark, Space, Odd, even, none   |             |             |             |             |
| Transmission rates :  |      | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |             |             |             |             |
| Handshake mode  |      | None   |             |             |             |             |

## Precision Balances

| Model  |     | CY 123   | CY 223                 | CY 323      | CY 363      | CY 423      | CY 623      | CY 723      | CY 1003     |
|--|-----|--|------------------------|-------------|-------------|-------------|-------------|-------------|-------------|
| Weighing Capacity                                | g   | 120  | 220                    | 320         | 360         | 420         | 620         | 720         | 1000        |
| Readability (d)                                  | g   | 0.001  | 0.001                  | 0.001       | 0.001       | 0.001       | 0.001       | 0.001       | 0.001       |
| Accuracy (e)                                     | g   | 0.01   | 0.01                   | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        |
| Tare Range (Subtractive)                         | g   | -120   | -220                   | -320        | -360        | -420        | -620        | -720        | -1000       |
| Repeatability (std. deviation)                   | <=g | 0.001  | 0.001                  | 0.001       | 0.001       | 0.001       | 0.002       | 0.002       | 0.002       |
| Linearity  | <=g | 0.002  | 0.002                  | 0.002       | 0.002       | 0.002       | 0.003       | 0.003       | 0.003       |
| Weighing Class                                   |     | II   | II                     | II          | II          | II          | II          | I           | I           |
| Response time (average)                          | s   | 2 - 3 sec.   |                        |             |             |             |             |             |             |
| Operating temperature range                      | °C  | 15° to 30°C  | 15° to 30°C            | 15° to 30°C | 15° to 30°C | 15° to 30°C | 15° to 30°C | 18° to 30°C | 18° to 30°C |
| Calibration                                      | °C  | External   | External               | External    | External    | External    | External    | External    | External    |
| External cal. wt. (of at least accuracy class..) | g   | 50 (F1)  | 100 (F1)               | 200 (F1)    | 200 (F1)    | 200 (F1)    | 300 (F1)    | 500 (F1)    | 500 (F1)    |
| Net Weight, approx.                              | kg  | 7.5kg  |                        |             |             |             |             |             |             |
| Pan size   | mm  | 128 x 128  |                        |             |             |             |             |             |             |
| Weighing chamber height with draftshield         | mm  | 158.5  |                        |             |             |             |             |             |             |
| Weighing chamber height with Windshield          | mm  | 81   |                        |             |             |             |             |             |             |
| Dimensions (W x D x H) with draftshield          | mm  | 342.5 x 212 x 271  |                        |             |             |             |             |             |             |
| Dimensions (W x D x H) with windshield           | mm  | 342.5 x 212 x 193.5  |                        |             |             |             |             |             |             |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             |             |             | ⊕           | ⊖           |
| Frequency  | Hz  | 50 / 60Hz  |                        |             |             |             |             |             |             |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |                        |             |             |             |             |             |             |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight                         |                        |             |             |             |             |             |             |
|  |     | carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels                   |                        |             |             |             |             |             |             |
|  |     | Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |             |             |             |             |
| Built-in-interface                               |     | RS-232/USB   |                        |             |             |             |             |             |             |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits                                   |                        |             |             |             |             |             |             |
| Parity   |     | Mark, Space, Odd, even, none   |                        |             |             |             |             |             |             |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud                                  |                        |             |             |             |             |             |             |
| Handshake mode                                   |     | None   |                        |             |             |             |             |             |             |

## Precision Balances

| Model  |     | CY 123C  | CY 223C                | CY 323C     | CY 363C     | CY 423C     | CY 623C     | CY 723C     | CY 1003C    |
|--|-----|--|------------------------|-------------|-------------|-------------|-------------|-------------|-------------|
| Weighing Capacity                                | g   | 120  | 220                    | 320         | 360         | 420         | 620         | 720         | 1000        |
| Readability (d)                                  | g   | 0.001  | 0.001                  | 0.001       | 0.001       | 0.001       | 0.001       | 0.001       | 0.001       |
| Accuracy (e)                                     | g   | 0.01   | 0.01                   | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        |
| Tare Range (Subtractive)                         | g   | -120   | -220                   | -320        | -360        | -420        | -620        | -720        | -1000       |
| Repeatability (std. deviation)                   | <=g | 0.001  | 0.001                  | 0.001       | 0.001       | 0.001       | 0.002       | 0.002       | 0.002       |
| Linearity  | <=g | 0.002  | 0.002                  | 0.002       | 0.002       | 0.002       | 0.003       | 0.003       | 0.003       |
| Weighing Class                                   |     | II   | II                     | II          | II          | II          | II          | I           | I           |
| Response time (average)                          | s   | 2 - 3 sec.   |                        |             |             |             |             |             |             |
| Operating temperature range                      | °C  | 15° to 30°C  | 15° to 30°C            | 15° to 30°C | 15° to 30°C | 15° to 30°C | 15° to 30°C | 18° to 30°C | 18° to 30°C |
| Calibration                                      | °C  | Internal   | Internal               | Internal    | Internal    | Internal    | Internal    | Internal    | Internal    |
| External cal. wt. (of at least accuracy class..) | g   | 50 (F1)  | 100 (F1)               | 200 (F1)    | 200 (F1)    | 200 (F1)    | 300 (F1)    | 500 (F1)    | 500 (F1)    |
| Net Weight, approx.                              | kg  | 7.8kg  |                        |             |             |             |             |             |             |
| Pan size   | mm  | 128 x 128  |                        |             |             |             |             |             |             |
| Weighing chamber height with draftshield         | mm  | 158.5  |                        |             |             |             |             |             |             |
| Weighing chamber height with Windshield          | mm  | 81   |                        |             |             |             |             |             |             |
| Dimensions (W x D x H) with draftshield          | mm  | 342.5 x 212 x 271  |                        |             |             |             |             |             |             |
| Dimensions (W x D x H) with windshield           | mm  | 342.5 x 212 x 193.5  |                        |             |             |             |             |             |             |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             |             |             | ⊕           | ⊖           |
| Frequency  | Hz  | 50 / 60Hz  |                        |             |             |             |             |             |             |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |                        |             |             |             |             |             |             |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight                         |                        |             |             |             |             |             |             |
|  |     | carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels                   |                        |             |             |             |             |             |             |
|  |     | Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |             |             |             |             |
| Built-in-interface                               |     | RS-232/USB   |                        |             |             |             |             |             |             |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits                                   |                        |             |             |             |             |             |             |
| Parity   |     | Mark, Space, Odd, even, none   |                        |             |             |             |             |             |             |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud                                  |                        |             |             |             |             |             |             |
| Handshake mode                                   |     | None   |                        |             |             |             |             |             |             |

## Top Loading Precision Balances

| Model  |     | CY 612   | CY 1202     | CY 3101     | CY 3102DR   | CY 4101     | CY 4102DR   | CY 6101     | CY 8101     |  |  |
|--|-----|--|-------------|-------------|-------------|-------------|-------------|-------------|-------------|--|--|
| Weighing Capacity                                | g   | 610  | 1200        | 3100        | 3100        | 4100        | 4100        | 6100        | 8100        |  |  |
| Readability (d)                                  | g   | 0.01   | 0.01        | 0.1         | 0.01        | 0.1         | 0.01        | 0.1         | 0.1         |  |  |
| Accuracy (e)                                     | g   | 0.1  | 0.1         | 1           | 0.1         | 1           | 0.1         | 1           | 1           |  |  |
| Tare Range (Subtractive)                         | g   | -610   | -1200       | -3100       | -3100       | -4100       | -4100       | -6100       | -8100       |  |  |
| Repeatability (std. deviation)                   | <=g | 0.01   | 0.01        | 0.1         | 0.01        | 0.1         | 0.01        | 0.2         | 0.3         |  |  |
| Linearity  | <=g | 0.02   | 0.02        | 0.2         | 0.02        | 0.2         | 0.02        | 0.3         | 0.4         |  |  |
| Weighing Class                                   |     | III  | II          | III         | II          | III         | II          | II          | II          |  |  |
| Response time (average)                          | s   | 2 - 3 sec.   |             |             |             |             |             |             |             |  |  |
| Operating temperature range                      | °C  | 15° to 45°C  | 15° to 30°C |  |  |
| Calibration                                      |     | External   | External    | External    | External    | External    | External    | External    | External    |  |  |
| External cal. wt. (of at least accuracy class..) | g   | 300 (F1)   | 1000 (F1)   | 1500 (F1)   | 1000 (F1)   | 2000 (F1)   | 1000 (F1)   | 4000 (F1)   | 5000 (F1)   |  |  |
| Net Weight, approx.                              | kg  | 5.5kg  |             |             |             |             |             |             |             |  |  |
| Pan size   | mm  | 198 x 205  | 198 x 205   | 198 x 205   | 198 x 205   | 198 x 205   | 198 x 205   | 198 x 205   | 198 x 205   |  |  |
| Dimensions (W x D x H)                           | mm  | 342.5 x 212 x 89.5   |             |             |             |             |             |             |             |  |  |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240 0.8A output 12V / 0.9A   |             |             |             |             |             | ⊕ - ⊖       |             |  |  |
| Frequency  | Hz  | 50 / 60Hz  |             |             |             |             |             |             |             |  |  |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |             |             |             |             |             |             |             |  |  |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |             |             |             |             |             |             |             |  |  |
| Built-in-interface                               |     | RS-232/USB   |             |             |             |             |             |             |             |  |  |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |             |             |             |             |             |             |             |  |  |
| Parity   |     | Mark, Space, Odd, even, none   |             |             |             |             |             |             |             |  |  |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |             |             |             |             |             |             |             |  |  |
| Handshake mode                                   |     | None   |             |             |             |             |             |             |             |  |  |

## Top Loading Precision Balances

| Model  |     | CY 2202  | CY 2202DR              | CY 3102     | CY 4102     | CY 6102   |
|--|-----|--|------------------------|-------------|-------------|---|
| Weighing Capacity                                | g   | 2200   | 200 / 2200             | 3100        | 4100        | 6100  |
| Readability (d)                                  | g   | 0.01   | 0.001 / 0.01           | 0.01        | 0.01        | 0.01  |
| Accuracy (e)                                     | g   | 0.1  | 0.01 / 0.1             | 0.1         | 0.1         | 0.1   |
| Tare Range (Subtractive)                         | g   | -2200  | -200 / 2200            | -3100       | -4100       | -6100   |
| Repeatability (std. deviation)                   | <=g | 0.01   | 0.002 / 0.02           | 0.01        | 0.01        | 0.02  |
| Linearity  | <=g | 0.02   | 0.003 / 0.03           | 0.02        | 0.02        | 0.03  |
| Weighing Class                                   |     | II   | I                      | II          | II          | I   |
| Response time (average)                          | s   | 2 - 3 sec.   |                        |             |             |   |
| Operating temperature range                      | °C  | 15° to 30°C  | 18° to 30°C            | 15° to 30°C | 15° to 30°C | 18° to 30°C   |
| Calibration                                      |     | External   | External               | External    | External    | External  |
| External cal. wt. (of at least accuracy class..) | g   | 1000 (F1)  | 1000 (F1)              | 1500 (F1)   | 2000 (F1)   | 4000 (F1)   |
| Net Weight, approx.                              | kg  | 5.5kg  |                        |             |             |   |
| Pan size   | mm  | 198 x 205  | 128 x 128              | 198 x 205   | 198 x 205   | 198 x 205   |
| Dimensions (W x D x H)                           | mm  | 342.5 x 212 x 89.5   |                        |             |             | 342.5 x 212 x 271   |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             |  |
| Frequency  | Hz  | 50 / 60Hz  |                        |             |             |   |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |                        |             |             |   |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |   |
| Built-in-interface                               |     | RS-232/USB   |                        |             |             |   |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |                        |             |             |   |
| Parity   |     | Mark, Space, Odd, even, none   |                        |             |             |   |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |                        |             |             |   |
| Handshake mode                                   |     | None   |                        |             |             |   |

## Top Loading Precision Balances

| Model  |     | CY 3102C   | CY 4102C    | CY 6102C    | CY 8102C    |
|--|-----|--|-------------|-------------|-------------|
| Weighing Capacity                                | g   | 3100   | 4100        | 6100        | 8100        |
| Readability (d)                                  | g   | 0.1  | 0.1         | 0.1         | 0.1         |
| Accuracy (e)                                     | g   | 1  | 1           | 1           | 1           |
| Tare Range (Subtractive)                         | g   | -3100  | -4100       | -6100       | -8100       |
| Repeatability (std. deviation)                   | <=g | 0.1  | 0.1         | 0.2         | 0.3         |
| Linearity  | <=g | 0.2  | 0.2         | 0.3         | 0.4         |
| Weighing Class                                   |     | III  | III         | II          | II          |
| Response time (average)                          | s   | 2 - 3 sec.   |             |             |             |
| Operating temperature range                      | °C  | 15° to 45°C  | 15° to 30°C | 15° to 30°C | 15° to 30°C |
| Calibration                                      |     | Internal   | Internal    | Internal    | Internal    |
| External cal. wt. (of at least accuracy class..) | g   | 1500 (F1)  | 2000 (F1)   | 4000 (F1)   | 5000 (F1)   |
| Net Weight, approx.                              | kg  | 6kg  |             |             |             |
| Pan size   | mm  | 198 x 205  |             |             |             |
| Dimensions (W x D x H)                           | mm  | 342.5 x 212 x 89.5   |             |             |             |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240 0.8A output 12V / 0.9A   |             | ⊕ ● ⊖       |             |
| Frequency  | Hz  | 50 / 60Hz  |             |             |             |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |             |             |             |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |             |             |             |
| Built-in-interface                               |     | RS-232/USB   |             |             |             |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |             |             |             |
| Parity   |     | Mark, Space, Odd, even, none   |             |             |             |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |             |             |             |
| Handshake mode                                   |     | None   |             |             |             |

## Top Loading Precision Balances

| Model  |     | CY 312C  | CY 612C     | CY1202C     | CY 2202C    | CY3102C     | CY 4102C    | CY 6102C    |  |
|--|-----|--|-------------|-------------|-------------|-------------|-------------|-------------|--|
| Weighing Capacity                                | g   | 310  | 610         | 1200        | 2200        | 3100        | 4100        | 6100        |  |
| Readability (d)                                  | g   | 0.01   | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        |  |
| Accuracy (e)                                     | g   | 0.1  | 0.1         | 0.1         | 0.1         | 0.1         | 0.1         | 0.1         |  |
| Tare Range (Subtractive)                         | g   | -310   | -610        | -1200       | -2200       | -3100       | -4100       | -6100       |  |
| Repeatability (std. deviation)                   | <=g | 0.01   | 0.01        | 0.01        | 0.01        | 0.01        | 0.01        | 0.02        |  |
| Linearity  | <=g | 0.02   | 0.02        | 0.02        | 0.02        | 0.02        | 0.02        | 0.03        |  |
| Weighing Class                                   |     | III  | III         | II          | II          | II          | II          | I           |  |
| Response time (average)                          | s   | 2 - 3 sec.   |             |             |             |             |             |             |  |
| Operating temperature range                      | °C  | 15° to 45°C  | 15° to 45°C | 15° to 30°C | 15° to 30°C | 15° to 30°C | 15° to 30°C | 18° to 30°C |  |
| Calibration                                      |     | Internal   | Internal    | Internal    | Internal    | Internal    | Internal    | Internal    |  |
| External cal. wt. (of at least accuracy class..) | g   | 200 (F1)   | 300 (F1)    | 1000 (F1)   | 1000 (F1)   | 1500 (F1)   | 2000 (F1)   | 4000 (F1)   |  |
| Net Weight, approx.                              | kg  | 6kg  |             |             |             |             |             |             |  |
| Pan size   | mm  | 198 x 205  |             |             |             |             |             |             |  |
| Dimensions (W x D x H)                           | mm  | 342.5 x 212 x 89.5   |             |             |             |             |             |             |  |
| DC power source / Power requirements             | V~  | DC Adapter, input 100 ~ 240 0.8A output 12V / 0.9A   |             |             |             |             |             | ⊕-●-⊖       |  |
| Frequency  | Hz  | 50 / 60Hz  |             |             |             |             |             |             |  |
| Power consumption (average)                      | VA  | maximum 18; typical 9  |             |             |             |             |             |             |  |
| Selectable weight units                          |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |             |             |             |             |             |             |  |
| Built-in-interface                               |     | RS-232/USB   |             |             |             |             |             |             |  |
| Format   |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |             |             |             |             |             |             |  |
| Parity   |     | Mark, Space, Odd, even, none   |             |             |             |             |             |             |  |
| Transmission rates :                             |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |             |             |             |             |             |             |  |
| Handshake mode                                   |     | None   |             |             |             |             |             |             |  |

## High Capacity Precision Balances

| Model   |     | CY 15001H  | CY 20001H              | CY 25001H   | CY 35001H   | CY 50001H   |
|---|-----|--|------------------------|-------------|-------------|-------------|
| Weighing Capacity                                       | Kg  | 15   | 20                     | 25          | 35          | 50          |
| Readability (d)   | g   | 0.1  | 0.1                    | 0.1         | 0.1         | 1           |
| Accuracy (e)  | g   | 1  | 1                      | 1           | 1           | 10          |
| Tare Range (Subtractive)                                | Kg  | -15  | -20                    | -25         | -35         | -50         |
| Repeatability (std. deviation)                          | <=g | 0.1  | 0.1                    | 0.1         | 0.1         | 1           |
| Linearity   | <=g | 0.2  | 0.2                    | 0.2         | 0.2         | 2           |
| Weighing Class  |     | II   | II                     | II          | II          | III         |
| Response time (average)                                 | s   | 2 - 3 sec.   |                        |             |             |             |
| Operating temperature range                             | °C  | 15° to 30°C  | 15° to 30°C            | 15° to 30°C | 15° to 30°C | 15° to 45°C |
| Calibration   |     | External   | External               | External    | External    | External    |
| External calibration weight (of at least acc. class...) | Kg  | 10 (F1)  | 10 (F1)                | 15 (F1)     | 15 (F1)     | 25 (F1)     |
| Net Weight, approx.                                     | kg  | 15kg   |                        |             |             |             |
| Pan size  | mm  | 400 x 300  |                        |             |             |             |
| Dimensions (W x D x H)                                  | mm  | 517 x 302 x 130  |                        |             |             |             |
| DC power source / Power requirements                    | V~  | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             | ⊕-●-⊖       |
| Frequency   | Hz  | 50 / 60Hz  |                        |             |             |             |
| Power consumption (average)                             | VA  | maximum 18; typical 9  |                        |             |             |             |
| Selectable weight units                                 |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |             |
| Built-in-interface                                      |     | RS-232/USB   |                        |             |             |             |
| Format  |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |                        |             |             |             |
| Parity  |     | Mark, Space, Odd, even, none   |                        |             |             |             |
| Transmission rates :                                    |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |                        |             |             |             |
| Handshake mode  |     | None   |                        |             |             |             |

## High Capacity Precision Balances

| Model   |     | CY 15001HC   | CY 20001HC  | CY 25001HC  | CY 35001HC  | CY 50001HC  |
|---|-----|--|-------------|-------------|-------------|-------------|
| Weighing Capacity                                       | Kg  | 15   | 20          | 25          | 35          | 50          |
| Readability (d)   | g   | 0.1  | 0.1         | 0.1         | 0.1         | 1           |
| Accuracy (e)  | g   | 1  | 1           | 1           | 1           | 10          |
| Tare Range (Subtractive)                                | Kg  | -15  | -20         | -25         | -35         | -50         |
| Repeatability (std. deviation)                          | <=g | 0.1  | 0.1         | 0.1         | 0.1         | 1           |
| Linearity   | <=g | 0.2  | 0.2         | 0.2         | 0.2         | 2           |
| Weighing Class  |     | II   | II          | II          | II          | III         |
| Response time (average)                                 | s   | 2 - 3 sec.   |             |             |             |             |
| Operating temperature range                             | °C  | 15° to 30°C  | 15° to 30°C | 15° to 30°C | 15° to 30°C | 15° to 45°C |
| Calibration   |     | Internal   | Internal    | Internal    | Internal    | Internal    |
| External calibration weight (of at least acc. class...) | Kg  | 10 (F1)  | 10 (F1)     | 15 (F1)     | 15 (F1)     | 25 (F1)     |
| Net Weight, approx.                                     | kg  | 15kg   |             |             |             |             |
| Pan size  | mm  | 400 x 300  |             |             |             |             |
| Dimensions (W x D x H)                                  | mm  | 517 x 302 x 130  |             |             |             |             |
| DC power source / Power requirements                    | V~  | DC Adapter, input 100 ~ 240 0.8A output 12V / 0.9A   |             |             |             | ⊕-●-⊖       |
| Frequency   | Hz  | 50 / 60Hz  |             |             |             |             |
| Power consumption (average)                             | VA  | maximum 18; typical 9  |             |             |             |             |
| Selectable weight units                                 |     | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |             |             |             |             |
| Built-in-interface                                      |     | RS-232/USB   |             |             |             |             |
| Format  |     | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |             |             |             |             |
| Parity  |     | Mark, Space, Odd, even, none   |             |             |             |             |
| Transmission rates :                                    |     | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |             |             |             |             |
| Handshake mode  |     | None   |             |             |             |             |

## Carat Balances

| Model   |      | CY 253K  | CY 603K                | CY 1503K    | CY 1603DR    |
|---|------|--|------------------------|-------------|--------------|
| Weighing Capacity   | ct   | 250  | 600                    | 1500        | 600/1600     |
| Readability (d)   | ct   | 0.001  | 0.001                  | 0.001       | 0.001/0.01ct |
| Accuracy (e)  | ct   | 0.01   | 0.01                   | 0.01        | 0.01         |
| Tare Range (Subtractive)                                    | ct   | -250   | -600                   | -1500       | -1600        |
| Repeatability (std. deviation)                              | <=ct | 0.001  | 0.001                  | 0.002       | 0.002        |
| Linearity   | <=ct | 0.002  | 0.002                  | 0.003       | 0.003        |
| Weighing Class  |      | II   | I                      | I           | I            |
| Response time (average)                                     | s    |  |                        |             |              |
| Operating temperature range                                 | °C   | 15° to 30°C  | 18° to 30°C            | 18° to 30°C | 18° to 30°C  |
| Calibration   |      | External   | External               | External    | External     |
| External calibration weight (of at least accuracy class...) |      | 25 (F1)  | 50 (F1)                | 200 (F1)    | 200 (F1)     |
| Net Weight, approx.   | kg   | 7.5  |                        |             |              |
| Pan size  | mm   | 90 Ø   |                        |             |              |
| Weighing chamber height                                     | mm   | 158.5  |                        |             |              |
| Dimensions (W x D x H)                                      | mm   | 342.5 x 212 x 271  |                        |             |              |
| DC power source / Power requirements                        | V~   | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             | ⊕—●—⊖        |
| Frequency   | Hz   | 50 / 60Hz  |                        |             |              |
| Power consumption (average)                                 | VA   | maximum 18; typical 9  |                        |             |              |
| Selectable weight units                                     |      | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong tales, Singapore taels<br>Taiwan tales, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |              |
| Built-in-interface  |      | RS-232/USB   |                        |             |              |
| Format  |      | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |                        |             |              |
| Parity  |      | Mark, Space, Odd, even, none   |                        |             |              |
| Transmission rates :  |      | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |                        |             |              |
| Handshake mode  |      | None   |                        |             |              |

## Carat Balances

| Model   |      | CY 103KC   | CY 253KC               | CY 603KC    | CY 1103KC   | CY 1503KC   |
|---|------|--|------------------------|-------------|-------------|-------------|
| Weighing Capacity   | ct   | 101  | 250                    | 600         | 1100        | 1500        |
| Readability (d)   | ct   | 0.001  | 0.001                  | 0.001       | 0.001       | 0.001       |
| Accuracy (e)  | ct   | 0.01   | 0.01                   | 0.01        | 0.01        | 0.01        |
| Tare Range (Subtractive)                                    | ct   | -101   | -250                   | -600        | -1100       | -1500       |
| Repeatability (std. deviation)                              | <=ct | 0.001  | 0.001                  | 0.001       | 0.001       | 0.002       |
| Linearity   | <=ct | 0.002  | 0.002                  | 0.002       | 0.002       | 0.003       |
| Weighing Class  |      | II   | II                     | I           | I           | I           |
| Response time (average)                                     | s    | 3 sec.   |                        |             |             |             |
| Operating temperature range                                 | °C   | 15° to 30°C  | 15° to 30°C            | 18° to 30°C | 18° to 30°C | 18° to 30°C |
| Calibration   |      | Internal   | Internal               | Internal    | Internal    | Internal    |
| External calibration weight (of at least accuracy class...) |      | 10 (F1)  | 25 (F1)                | 50 (F1)     | 100 (F1)    | 200 (F1)    |
| Net Weight, approx.   | kg   | 7.8kg  |                        |             |             |             |
| Pan size  | mm   | 90 Ø   |                        |             |             |             |
| Weighing chamber height                                     | mm   | 158.5  |                        |             |             |             |
| Dimensions (W x D x H)                                      | mm   | 342.5 x 212 x 271  |                        |             |             |             |
| DC power source / Power requirements                        |      | DC Adapter, input 100 ~ 240  | 0.8A output 12V / 0.9A |             |             | ⊕—●—⊖       |
| Frequency   | V~   | 50 / 60Hz  |                        |             |             |             |
| Power consumption (average)                                 | Hz   | maximum 18; typical 9  |                        |             |             |             |
| Selectable weight units                                     |      | gram, kilogram, pound, ounce, troy ounce, grain, pennyweight<br>carat, Milligram, momme, mesghal, Hong Kong taels, Singapore taels<br>Taiwan taels, baht, Myanmar gold (mg <sup>1</sup> ), Myanmar gold (mg <sup>2</sup> ) |                        |             |             |             |
| Built-in-interface  |      | RS-232/USB   |                        |             |             |             |
| Format  |      | 1 start bit, 8-bit ASCII, parity, 1 or 2 stop bits   |                        |             |             |             |
| Parity  |      | Mark, Space, Odd, even, none   |                        |             |             |             |
| Transmission rates :  |      | 300; 600; 1200; 2400; 4800; 9600; 19200; 57600 baud  |                        |             |             |             |
| Handshake mode  |      | None   |                        |             |             |             |

## 14. Accessories (Option)

**Statistical Printer "CPR 02"**  
with Date / Time & Statistics

**Remote Display "SRD01"**

**Calibration Weights**  
(F1) (ERTL, F2 with certificate) for further details, contact ACZET Dealers.

**USB Interface**

**Density Kit "CDK 01"**  
For determination of solids for determination of liquids with displacement body

**Antitheft device**  
Cable and lock (for all models)

**Dust Cover**

**Evaporation Trap kit "CET 01"**  
For Analytical Balances get accurate pipette testing/calibration  
minimizes errors caused by evaporation

Subject to technical changes and to the availability  
of the accessories supplied with the instruments.

#### **INDIA**

**Aczet Pvt. Ltd.**  
E-2, Plot No. 15, WICEL,  
Opp. Seepz Gate No. 1,  
Andheri (E), Mumbai 400093.  
Email : [export@aczet.com](mailto:export@aczet.com)  
[sales@aczet.com](mailto:sales@aczet.com)  
Toll Free No. 022 42437700

#### **USA**

**Aczet INC.**  
1637, Stelton Road Unit B-5,  
Piscataway, NJ 08854  
Email : [tejas@aczet.com](mailto:tejas@aczet.com)  
Toll Free : 1800 997 1440

#### **UAE**

**Aczet Instruments LLC**  
P.O.Box 27137, Old Goldsouq,  
Deira - Dubai.  
Email : [danny.s@aczet.com](mailto:danny.s@aczet.com)  
Phone : +971 50 6593253

#### **THAILAND**

**Aczet Thailand Co. Ltd.**  
1A1, Gr. Floor, BIS Building,  
119 Mahesak Road, Suryawong,  
Bangrak, Bangkok - 10500  
Email : [utkarsh.p@aczet.com](mailto:utkarsh.p@aczet.com)  
Phone : +66 920456757