


Operating Instructions

Sartorius Moisture Analyzer

Model MA35 Electronic Moisture Analyzer



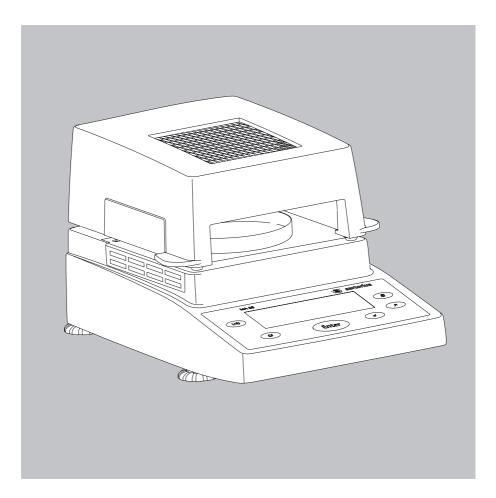

Intended Use

Contents

The MA35 moisture analyzer is
intended for fast and reliable deter-
mination of the moisture content
of materials of liquid, pasty and solid
substances using the thermogravi-
metric method.

Symbols

The following symbols are used in these instructions:

- indicates steps you must perform
- indicates steps required only under certain conditions
- describes what happens after you have performed a particular step
- indicates an item in a list



Intended Use
Warnings and Safety Information 3
Getting Started6General View of the Equipment6Equipment Supplied7Connecting the Moisture Analyzer
to AC Power
Operating Design 13 Keys 13 Display 14
Configuration15Setting the Device Parameters15Setting the Drying Parameters17
Operation21Example: Analysis with SpecifiedDrying Time21
Adjusting the Analyzer
Interface Port 26 Pin Assignments 27
Error Codes
Care and Maintenance
Overview. 32 Specifications. 32 Accessories (Options) 33 Declaration of Conformity. 34

Warnings and Safety Information

This moisture analyzer complies with the European Council Directives as well as international regulations and standards for electrical equipment, electromagnetic compatibility, and the stipulated safety requirements. Improper use or handling, however, can result in damage and/or injury.

To prevent damage to the equipment, read these operating instructions thoroughly before using your MA35 moisture analyzer. Keep these instructions in a safe place.

Follow the instructions below to ensure safe and trouble-free operation of your moisture analyzer:



\ Use the moisture analyzer only for performing moisture analysis on samples. Any improper use of the analyzer can endanger persons and may result in damage to the analyzer or other material assets.



/!\ Do not use this moisture analyzer in a hazardous area; operate it only under the ambient conditions specified in these instructions.



/!\ If you use electrical equipment in installations and under ambient conditions subject to stricter safety standards than those described in the manual, you must comply with the provisions as specified in the applicable regulations for installation in your country.

The moisture analyzer may be operated only by qualified persons who are familiar with the properties of the sample to be analyzed.



/!\ Make sure before getting started that the voltage rating printed on the manufacturer's label is identical to your local line voltage (see "Connecting the Moisture Analyzer to AC Power" in the chapter entitled "Getting Started").

- The analyzer comes with a power supply that has a grounding conductor.
- The only way to switch the power off completely is to unplug the power cord.
- Position the power cord so that it cannot touch any hot areas of the moisture analyzer.
- Use only extension cords that meet the applicable standards and have a protective grounding conductor.
- Disconnecting the ground conductor is prohibited.
- Connect only Sartorius accessories and options, as these are optimally designed for use with your moisture analyzer.

Note on installation:

The operator shall be responsible for any modifications to Sartorius equipment or connections of cables not supplied by Sartorius and must check and, if necessary, correct these modifications. On request, Sartorius will provide information on the minimum operating specifications (in accordance with the Standards listed on p. 33 for defined immunity to interference).

- Protect the analyzer from contact with liquid
- If there is visible damage to the equipment or power cord, unplug the equipment and lock it in a secure place to ensure that it cannot be used for the time being.

/!\ Clean your moisture analyzer only according to the cleaning instructions (see "Care and Maintenance").

Do not open the analyzer housing. If the seal is broken, this will result in forfeiture of all claims under the manufacturer's warranty.

If you have any problems with your moisture analyzer:

contact your local Sartorius office, dealer or service center



Warning: Severe Burns!

- When setting up the moisture analyzer. leave enough space to prevent heat from building up and to keep your analyzer from overheating:
 - leave 20 cm (about 8 inches) around the moisture analyzer
 - leave 1 m (3 ft.) above the moisture analyzer
- Do not place any flammable substances on, under or near the moisture analyzer, because the area around the heating unit will heat up
- Be careful when removing a sample from the chamber: the sample, the heating unit and the sample pan may still be extremely hot
- Prevent excess heat build-up around the analyzer

Hazards for persons or equipment posed by certain sample materials:





Fire

Explosion

- Flammable or explosive substances
- Substances that contain solvents
- Substances that release flammable or explosive gases or vapors during the drying process

In some cases, it is possible to operate the moisture analyzer in an enclosed nitrogen atmosphere to prevent the vapor released during drying from coming into contact with oxygen in the surrounding atmosphere. Check on a case-to-case basis whether this method can be used, because installation of the analyzer in too small an enclosed space can affect its functioning (for instance, through excessive heat build-up within the analyzer). When in doubt, perform a risk analysis.

The user shall be liable and responsible for any damage that arises in connection with this moisture analyzer.





Poisoning

Caustic burns

 Substances containing toxic or caustic or corrosive components may only be dried under a fume hood. The value for the "lower toxic limit" in a work area must not be exceeded.

Corrosion:


 Corrosion may be caused by substances that release aggressive vapors during the heating process (such as acids).

We recommend working with only small quantities of such samples, to avoid build-up of vapors that can condense on cold housing parts and can cause corrosion.

The user shall be liable and responsible for any damage that arises in connection with this moisture analyzer.

Getting Started

General View of the Equipment

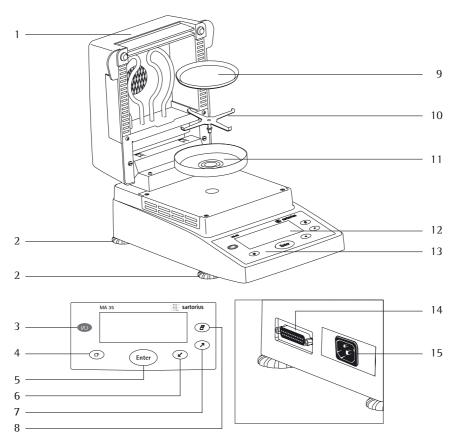

Pos.	Designation
1	Hinged cover with heating element
2	Leveling feet
3	On/off key
4	CF key (clear function; delete)
5	Enter key (confirm)
6	'Down/Back' key
7	'Up/Forward' key
8	Print key

Pos.	Designation
9	Disposable sample pan
10	Pan support
11	Pan draft shield
12	Display
13	Keypad
14	Interface port
15	Power jack

The moisture analyzer consists of a heating unit, a weighing system, and a display and control unit. In addition to the socket for AC power (mains supply), it also has an interface port for connecting peripheral devices, such as a computer, printer, etc.

Storage and Shipping Conditions Allowable storage temperature: 0 to 40°C: 32 to 104°F

Do not expose the moisture analyzer unnecessarily to extreme temperatures, moisture, shocks, blows or vibration.

Unpacking the Moisture Analyzer

- After unpacking the equipment, please check it immediately for any visible damage
- If any sign of damage is visible, proceed as directed under "Safety Inspection" in the chapter entitled "Care and Maintenance."

It is a good idea to save the box and all parts of the packaging until you have successfully installed your equipment. Only the original packaging provides the best protection for shipment. Before packing your moisture analyzer, unplug all connected cables to prevent damage.

Equipment Supplied

The equipment supplied includes the components listed below:

- Moisture analyzer
- Power cord
- Pan support
- Pan draft shield
- 80 disposable aluminum sample pans
- 1 pair of forceps

Installation Instructions

The MA35 moisture analyzer is designed to provide reliable results under normal ambient conditions in the laboratory and in industry. When choosing a location to set up your analyzer, observe the following so that you will be able to work with added speed and accuracy:


- Set up the moisture analyzer on a stable, even surface that is not exposed to vibrations, and level it using the four leveling feet
- Avoid placing the moisture analyzer in close proximity to a heater or otherwise exposing it to heat or direct sunlight
- Avoid exposing the moisture analyzer to extreme temperature fluctuations
- Protect the moisture analyzer from drafts that come from open windows or doors
- Keep the moisture analyzer protected from dust, whenever possible
- Protect the moisture analyzer from aggressive chemical vapors
- Do not expose the equipment to extreme moisture over long periods
- Make sure to choose a place where excessive heat cannot build up.
 Leave enough space between the moisture analyzer and materials that are affected by heat.

Conditioning the Moisture Analyzer

Moisture in the air can condense on the surfaces of a cold moisture analyzer whenever it is brought into a substantially warmer place. If you transfer the moisture analyzer to a warmer area, condition it for about 2 hours at room temperature, leaving it unplugged from AC power. Afterwards, if you keep the moisture analyzer connected to AC power, the constant positive difference in temperature between the inside of the equipment and the outside will practically rule out the effects of moisture condensation.



- Position the components listed below in the order given:
- Pan draft shield
- Pan support
- Disposable sample pan



Connecting the Moisture Analyzer to AC Power


- Check the voltage rating and the plug design
- The heating element has been factory-set to 230 V or 115 volts for technical reasons. The voltage has been set as specified on your order. The voltage setting is indicated on the manufacturer's label (see the bottom of the analyzer), for example:
 - 230 volts: MA35-...230...
 - 115 volts: MA35-...115...



If the voltage indicated on the label does not match your local line voltage:

Do not operate your moisture analyzer; contact your local Sartorius office or dealer.
Use only

- Genuine Sartorius power cords, or
- Power cords approved by a certified electrician
- If you need to connect an extension cord, use only a cable with a protective grounding conductor





If you use an electrical outlet that does not have a protective grounding conductor, make sure to have an equivalent protective conductor installed by a certified electrician as specified in the applicable regulations for installation in your country. Make sure the protective grounding effect is not neutralized by use of an extension cord that lacks a protective grounding conductor.



Connecting Electronic Peripheral Devices

 Make absolutely sure to unplug the analyzer from AC power before you connect or disconnect a peripheral device (printer or PC) to or from the interface port. NOTE: This equipment has been tested and found to comply with the limits pursuant to part 15 of FCC Rules.

These limits are designed to provide reasonable protection against harmful interference. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with these instructions, may cause harmful interference to radio communications.


For information on the specific limits and class of this equipment, please refer to the Declaration of Conformity. Depending on the particular class, you are either required or requested to correct the interference.


If you have a Class A digital device, you need to comply with the FCC statement as follows: "Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense."


If you have a Class B digital device, please read and follow the FCC information given below: "However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help."

Before you operate this equipment, check which FCC class (Class A or Class B) it has according to the Declaration of Conformity included. Be sure to observe the information of this Declaration







Warmup Time

To deliver exact results, the moisture analyzer must warm up for at least 30 minutes every time you connect it to AC power or after a relatively long power outage.

Only after this time will the analyzer have reached the required operating temperature.

Leveling the Moisture Analyzer

Purpose:


- To compensate for unevenness at the place of installation
- This is particularly important for testing liquid samples, which must be at a uniform level in the sample pan

Always level the moisture analyzer again any time after it has been moved to a different location.

 Extend or retract the front and/or rear leveling feet as needed to adjust the moisture analyzer

Installing the Aluminum Panels (Optional; Part No. YDS05MA)

- ∧ To prevent burns, allow the glass panels to cool sufficiently before removing them
- ▲ Do not scratch the aluminum panels; do not use abrasive or corrosive substances to clean the aluminum panels
- Remove the 2 rubber caps and the 2 screws beneath them, and then remove the panel retainer
- Remove the glass panels
- Position the aluminum panels in the retainer
- Fasten the aluminum panels with the retainer and screws; replace the 2 rubber caps




Turning On the Analyzer; Opening and Closing the Sample Chamber

- To turn on the analyzer: press 🗥
- When opening or closing the sample chamber, do not release the cover until it is in the fully open or fully closed position

Operating Design

Operation of the moisture analyzer follows a standardized "philosophy" which is described below.

There is only one key to a function, i.e., the key retains this function throughout most of the menu levels. The texts and symbols shown always have the same meaning.



Keys

Some of the keys trigger different functions, depending on whether you press the key briefly or press and hold the key:


- Press briefly = hold the key down for less than 1.2 seconds
- Press and hold = hold the key down for more than 1.2 seconds
- If you press and hold longer than 1.2 seconds, the function triggered is repeated every 0.6 seconds for as long as you hold the key.

Key	Designation	Press briefly	Press and hold
(1/0)	On/off key	Switch device on or off*	_
CF	CF key	Analysis: cancel function Menu: cancel selection	-
Enter	Enter key	Analysis: trigger the selected function (e.g., Menu: store the selected setting	Menu: store the selected setting and tare) close the menu
V	Down/Back key	Analysis: select a function (e.g., tare) Menu: decrease value or return to previous selection	Menu: decrease value 10-fold
P	Up/Forward key	Analysis: select a function (e.g., tare) Menu: increase value or go to next selection	Menu: increase value 10-fold
(I)	Print key	Send readout value or data record over the interface port	-

^{*} When you switch off the moisture analyzer, it remains in standby mode

Display

The texts and symbols shown on the display always have the same meaning. The display is divided into several areas.



Drying parameters:

The following symbols indicate drying program parameters for information, selection and configuration:



120°C Target temperature



☐ Yūmin Drying time Fully automatic



Weight unit or unit for a calculated value



Analysis start



2.0min Interval for automatic output of intermediate

results

Adjustment function:



Busy symbol, plus/minus sign, standby symbol:

The **o** symbol is shown here when the moisture analyzer is processing a function. The plus/minus sign for the weight value or calculated value appears here as well, and the standby symbol when the device is switched off.

Result:

This section shows the weight or calculated

Unit:

When the weighing system stabilizes, the unit of measurement for the weight or calculated value is displayed here.

Graphic symbols:

Which symbol is shown here depends on the operating status of the analyzer. The examples below indicate "Please close hood," "Heating the sample" and "Please wait" (hourglass).









Function line:


Press the Down/Back or Up/Forward keys to move the focus and select one of the functions shown here, and the Enter key to activate the selected function:

END START CAL SET PRG TAR

Configuration

Setting the Device Parameters

- o Factory setting
- √ User-defined setting

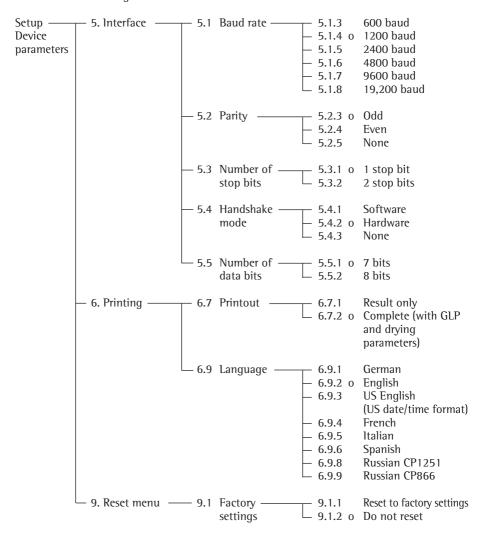


Example Changing the language to US mode (menu item 6.9.3)

Step	Key (or instruction)	Display
1. Select SET in the function line	Repeatedly:	1 :20°C ⊙ R +
2. Confirm SET	Enter	5.
3. Select menu item 6	7	Б.
4. Open submenu	Enter	5.7
5. Select menu item 6.9	7	6.9
6. Open submenu	Enter	6.9.2°
7. Select menu item 6.9.3	V	6.9.3
8. Confirm menu item 6.9.3	Enter	6.9.3°
9. Close the Setup menu	Repeatedly: CF	‡ :20°C ⊙ R + 0000 g

Setting the Drying Parameters

Select PRG in the function line to adapt parameters for the drying program to the particular requirements of the product sampled.

Drying Parameters

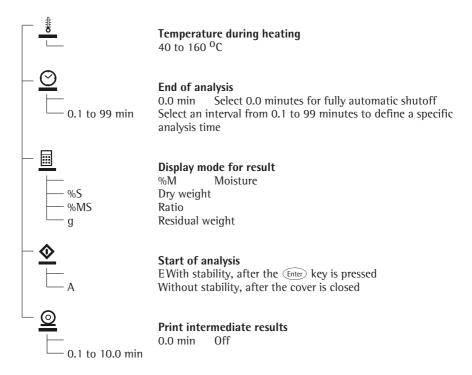

Features

Temperature during heating

Adjusted to defined specified temperature during the analysis process

Start of analysis

- With stability after the Enter key is pressed:

When START is shown in the function line and you press (Enter) to confirm, the initial weight is stored at stability regardless of whether the cover is open or closed.

Measurement begins as soon as the cover is closed.

Without stability after the cover is closed:


A symbol shown in the graphic symbol display prompts you to close the cover once the initial weight condition is met. The initial weight is stored without stability as soon as the sample chamber is closed, and analysis begins.

End of Analysis with Shutoff Parameters

- Fully automatic mode
- Timer mode

Fully automatic mode:

Use the fully automatic mode when loss of weight on drying follows a clearly delineated curve which can be unambiquously evaluated (see below).



Timer mode:

The analysis ends as soon as the specified time has elapsed.

Display Mode for Result

The following units can be selected for displaying analysis results:

Moisture %MDry weight %SRatio %MSResidual weight q

Print Intermediate Results

Intermediate results can be printed either at user-definable intervals or by pressing the (2) key.

Example: setting the following drying parameters Final temperature: 130 °C Start of analysis: without stability after the cover is closed End of analysis: after 10 minutes Display mode for result: moisture

Step	Key (or instruction)	Display
1. Turn on the analyzer	(VO)	Self-test runs
		\$ 105°C ⊙ R +
2. Select PRG: drying program parameters	V	PRG
3. Confirm PRG (the previously set temperature is displayed; in this example, 105°C)	Enter	<u></u>
4. Set the heating temperature (in this example: 130°C)	repeatedly	<u></u> i∃0°C
5. Confirm heating temperature (the previously set analysis time is displayed; in this example, 0.0 min)	Enter	<u>○</u> 0.0 min
6. Set the parameter for the end of analysis; in this example, 10 minutes)	repeatedly	<u></u> □ min
7. Confirm the "end of analysis" parameter	Enter	<u> </u>
8. Select the result display mode (in this example, moisture)	? or v	% M

Step)	Key (or instruction)	Display
9.	Confirm the display mode	Enter	◆ _E
10.	Select the start parameter (in this example, W/o stability after the cover is closed)		◆ A
11.	Confirm the start parameter	Enter	<u>⊚</u> 10 min
12.	Select setting for printout of intermediate results (in this example, no printout = 0.0)	v repeatedly	<u>◎</u> 0.0 min
13.	Confirm setting for intermediate printout of results	Enter	<u></u>
14.	Save changes and exit menu for drying parameter input	(Enter) > 2 sec	\$ 130°C ⊙ 10min +

Operation

Example: Analysis with Specified Drying Time

The specified drying time in the example is 10 minutes.

Final temperature: 130 °C

Start of analysis: Without stability after the cover is closed

End of analysis: After 10 minutes

Display mode: Moisture

Step Key (or instruction) Display 1. Switch on the moisture (1/0) Self-test runs analyzer 1 105°C ⊙ B CAL SET PRG 2. Set the drying parameters (see "Setting the Drying Parameters" in the chapter entitled "Configuration") 3. Open the sample chamber and place an unused sample pan on the pan support 130°C ♥ 10min 4. Tare the sample pan: select TAR as needed ...and confirm (Enter) 5. Distribute approx. 2 g sample 130°C ⊙ 10min evenly on the sample pan 6. Close the sample chamber 130°C ⊙ 10min The printout header is printed: see next page

Step

Key (or instruction) Display

The printout header is printed

*) Date and time included only if a Sartorius printer model YDP02 or YDP03 is used

Current moisture loss and elapsed time are displayed (in this example, 0.36% moisture after 0.3 min)

Drying stops automatically after 10 minutes

The footer of the printout is printed

You can print the result as often as you wish by pressing ②
Printout when function canceled: ("B" stands for "Break")

7. Clear the display

During and after the analysis you can change the mode for display and printout of results at any time by pressing the 🔑 and 🕜 keys.

23.08.2005 11:25 *)

Model MA35-000230V1 Ser. no. 99992581 Ver. no. 00-33-01

ΙD

Temp. 130 'C Start W/O STABI. End 10.0 min

IniWt + 2.036 g





10.0 + 10.90 %M FinWt + 1.814 g

Name:

10.0 + 10.90 %M

B 5.7 + 0.03 %M

(Enter)

Adjusting the Analyzer

Heating Element Adjustment

The procedure for adjusting the heating element is described in the instructions supplied with the YTM01MA temperature adjustment set.

Weighing System Adjustment

To adjust the weighing system, perform calibration and adjustment as described in the following.

Purpose

Calibration is the determination of the difference between the weight readout and the true weight (mass) of a sample. Calibration does not entail making any changes within the weighing system.

Adjustment is the correction of the difference between the measured value displayed and the true weight (mass) of a sample, or the reduction of the difference to a level within specified permissible error limits.

Features

Calibration is performed externally with the following weight value:

 MA35: 30 g; see "Accessories," order no. YSS43

You can have calibration and adjustment results documented as a ISO/GLPcompliant printout (see the page after next for an example).

External Calibration and Adjustment with a Factory-Defined Weight Externally calibrate and adjust the weighing system using a 30-g calibration weight.

Step	Key (or instruction)	Display
1. Turn on the analyzer	ON	Self-test runs # 130°C ⊙ R +
2. Select CAL for calibration/ adjustment	•	1 30°C ⊙ A + 0000 9 g CAL SET PRG TAR
3. Confirm CAL	Enter	Pb CAL
4. Confirm again when Pb is shown	Enter	+ 0009 g TAR
5. Tare the weighing system	Enter	Pb QQQ QQQ QQQ QQQ QQQ QQQ QQQ QQQ QQQ Q
6. Select CAL again	7	Pb OOD g TAR
7. Confirm CAL	Enter	Pb ◆

Key (or instruction) Display


The prompt for calibration weight is displayed



8. Open the hinged cover

Step

9. Place the 30-weight on the weighing system Minus sign –: weight value too low Plus sign +: weight value too high



The weight unit symbol (g) is displayed at the end of adjustment

Printout after calibration and adjustment

*) Date and time included only if a Sartorius printer model YDP02 or YDP03 is used





23.08.2005 10:51 *)
Model MA35-000230V1
Ser. no. 99992581
Ver. no. 00-33-01

External calibration W-ID
Nom. + 30.000 g
Diff. + 0.001 g
External adjustment

iff. + 0.000 g completed

0 0 ... p

Name:

- 10. Unload the analyzer
- 11. Quit calibration/adjustment

Close the cover



Interface Port

Purpose

The moisture analyzer has an interface port for connecting an external printer or computer (or other peripheral device).

External Printer You can use an external printer to generate printouts.

Computer

Analyses and calculated values can be transmitted to a computer for further evaluation and for documentation.

RS-232 cables purchased from other manufacturers often have pin assignments that are incompatible with Sartorius products. Be sure to check the pin assignments against the chart on the next page before connecting the cable, and disconnect any lines identified differently from those specified by Sartorius (e.g., pin 11). Failure to do so may damage or even completely ruin your moisture analyzer and/or peripheral device(s).

Preparation

For instructions on adapting the interface port to the peripheral device, please refer to the chapter entitled "Configuration."

To get the most from the versatile characteristics of your moisture analyzer with regard to documentation of results, we recommend connecting a printer from Sartorius. The resulting printouts will contribute decisively to simplifying GLP-compliant practices.

Female Interface Connector 25-position D-Submini (DB25S) with screw lock hardware for cable gland

Required Male Connector 25-pin D-Submini (DB25S) with shielded cable clamp assembly (Amp type 826 985-1C) and fastening screws (Amp type 164 868-1).

Pin assignments in the 25-contact

RS-232 female connector

Pin 1: Signal ground

Pin 2: Data output (TxD)

Pin 3: Data input (RxD)

Pin 4: Not connected

Pin 5: Clear to send (CTS)

Pin 6: Not connected

Pin 7: Internal ground (GND)

Pin 8: Not connected

Pin 9: Not connected

Pin 10: Not connected

Pin 11: Rechargeable battery: charge voltage

+10 V (1 _out 25 mA)

Pin 12: Reset _Out *)

Pin 13: +5 V output

Pin 14: Internal ground (GND)

Pin 15: Not connected Pin 16: Not connected

Pin 17: Not connected

Pin 18: Not connected

Pin 19: Not connected

Pin 20: Data terminal ready (DTR)

Pin 21: Not connected

Pin 22: Not connected

Pin 23: Not connected

Pin 24: Not connected

Pin 25: +5 V output

*) = Peripheral device restart



Error Codes

Error codes are displayed dynamically, for 2 seconds, or permanently. After a code is displayed dynamically or for 2 seconds, the program returns automatically to the normal operating mode.

Display	Cause	Solution
Н	The load exceeds the weighing	Unload the pan support capacity
L or Err54	Load is below the weighing range	Place the pan support on the weighing system
Err 0 I	Data output not compatible with output format	Change the configuration in the Setup menu
Err 02	Calibration/adjustment condition not met, e.g., – not tared – the pan support is loaded	Calibrate only when zero is displayed Select TAR to tare Unload the moisture analyzer
Err 03	Calibration/adjustment could not be completed within a certain time	Allow the scale to warm up again and repeat the adjustment
Err 30	Interface port for printer output is blocked	Have the port setting changed by Sartorius Customer Service
Err 3 I	Peripheral device not responding (interface handshake interrupted; XOFF, CTS)	Send XON, release CTS
Err 50	Temperature compensation overflow/underflow	Contact your local Sartorius Service Center
Err 53	Temperature compensation not functioning	Contact your local Sartorius Service Center
Err 55	Output from weighing ADC too high	Contact your local Sartorius Service Center
Err 79	Dryer adjustment data not found	Contact your local Sartorius Service Center
Err 24 I, Err 243	Weighing system parameters (EEPROM) defective	Switch the analyzer off and then on again. If the error persists, contact your local Sartorius Service Center
Err 2xx	Internal error	Contact your local Sartorius Service Center
Err 340	Operating parameters (EEPROM) incorrect	Contact your local Sartorius Service Center
Err 342	Operating parameters (EEPROM) incorrect except adjustment parameters	Contact your local Sartorius Service Center

If any other errors occur, contact your local Sartorius Service Center.

Contact information: Please point your Internet browser to: http://www.sartorius.com

Care and Maintenance

Service

Regular servicing by a Sartorius technician will extend the service life of your analyzer and ensure its continued accuracy of measurement. Sartorius can offer you service contracts, with your choice of regular maintenance intervals ranging from 1 month to 2 years.

The optimum length of the service interval depends on the operating conditions at the place of installation and on your requirements.

Repairs

Repair work must be performed by trained service technicians. Any attempt by untrained persons to perform repairs may result in considerable hazards for the user.



Cleaning

/!\ Make sure that no dust or liquid enters the moisture analyzer housing

- Do not use any aggressive cleaning agents (solvents, abrasive cleaning agents, etc.); clean the moisture analyzer using a piece of cloth which has been wet with a mild detergent (soap) only
- Disconnecting the power supply: unplug the power cord from the wall outlet (mains supply); if you have a cable connected to the interface, unplug it from the moisture analyzer
- The pan draft shield and the pan support can be removed for cleaning
- Carefully remove any sample residue/spilled powder using a brush or a handheld vacuum cleaner
- After cleaning, wipe down the analyzer with a soft, dry cloth




Cleaning the Heating Unit and Temperature Sensor


• Open the hinged cover

Danger: The terminals of the heating unit are under live current

 Disconnect the power supply by unplugging the power cord from the wall outlet (mains)
 If you have a cable connected to the interface port, disconnect it from the moisture analyzer



Carefully remove any residue from the temperature sensor



• Use a brush or a damp, lint-free cloth to clean the tubular metal heating element.

Safety Inspection

If there is any indication that safe operation of the equipment is no longer warranted:

- Disconnect the power supply by unplugging the power cord from the wall outlet (mains)
- Lock the equipment in a secure place to ensure that it cannot be used for the time being
 Safe operation of the equipment is no
- longer ensured when:there is visible damage to the device or power cord,
- the analyzer no longer functions properly.
- the equipment has been stored for a relatively long period under unfavorable conditions, or
- the equipment has been subjected to rough handling during shipment.

In this case, notify your nearest Sartorius Service Center. Maintenance and repair work may be performed only by service technicians who are authorized by Sartorius and who:

- have access to the required service and maintenance manuals, and
- have attended the relevant service training courses.

We recommend having the moisture analyzer inspected regularly according to the following checklist by a qualified Sartorius service technician:

- Resistance of the protective grounding conductor < 0.2 ohm measured with a commercially available multimeter
- Insulation resistance > 2 megaohms measured with a constant voltage of at least 500 volts at a 500 kohm load

A qualified Sartorius service technician should determine which tests are performed at what intervals, based on ambient and operating conditions. Inspections must be performed at least once a year.

Recycling



If you no longer need the packaging after successful installation of the equipment, you should return it for recycling. The packaging is made from environmentally

friendly materials and is a valuable source of secondary raw material. Batteries are hazardous waste and must be disposed of separately. Please deposit empty batteries in the collection boxes set up in your area for this purpose. On request, Sartorius can provide GRS boxes for collecting used batteries (GRS stands for "Gemeinsames Rücknahme System," a German organization for battery disposal). Contact your local waste disposal authorities if you wish to scrap the equipment. Remove batteries before scrapping the equipment. Sartorius in Goettingen will take back equipment and packaging for disposal in accordance with the applicable laws.*

* This service is offered only within Germany. If you set up the equipment in a country other than Germany, please contact your local waste disposal authorities for information on similar services.

Overview

Specifications

Weighing capacity (Max)	35 g
Accuracy of the weighing system	1 mg
Repeatability (average)	from about 1 g initial sample: \pm 0.2 % from about 5 g initial sample: \pm 0.05 %
Readability	0.01 %
Display of results	% moisture % dry weight % ratio g residual weight
Shutoff criteria	Fully automatic Timer mode: 0.1 to 99 min
Sample heating	Infrared radiation from a tubular metal heating element
Access to sample chamber	Flip-open cover with wide-angle opening
For conformity with FDA/HACCP regulations	Aluminum panels (in place of glass panels)
Operating temperature range and setting	40°C to 160°C (104°F to 320°F), adjustable in 1°C increments
Operator guidance	Symbols
Program memory capacity	1 program
Measured value memory capacity	Final value stored until subsequent measurement begins
Printout of measured values	Short printout GLP-compliant record in German, English, French, Italian, Spanish or Russian
Interface port	RS-232C, 25-pin connector for transfer of values to a printer or computer
Housing dimensions in mm	Width 224, depth 366, height 191
Net weight, approx.	5.8 kg
Power requirements (supply voltage):	230 V or 115 V (depending on the model) (–15% +10%); 50 – 60 Hz
Frequency	48 – 60 Hz
Fuses	2 (zero conductor/phase), 6.3 A, time-lag (slow-blow), 5×20 mm (internal)
Power consumption	400 VA
Ambient conditions: Operating temperature range:	+10 +30°C (+50° +86°F)
Allowable ambient operating temperature:	+5°C +40°C (+41°F +104 °F)
Ambient storage temperature:	−20°C +70°C (-4°F +158°F)
Relative humidity:	Up to 80% at $+31^{\circ}$ C (+ 88°F) ambient temperature; linearly decreasing down to 50% at $+40^{\circ}$ C ($+104^{\circ}$ F), non-condensing
Operating altitude	For use above sea level up to 2,000 m (6,562 feet); indoor use only

Accessories (Options)

Accessories	Order No.	
80 disposal sample pans	6965542	
Aluminum; 90 mm Ø		
80 glass fiber filters For liquid and pasty samples and samples with high fat-content	6906940	
Exchangeable panels for flip-open cover Replaces glass with aluminum panels for compliance with FDA/HACCP regulations (upgrade kit)	YDS05MA	
Model YDP20-0CE data printer for external connection	YDP20-0CE	
Color ink ribbon for YDP20-0CE data printer	6906918	
Paper for YDP20-0CE data printer; 5 rolls; length: 50 m	6906937	
External calibration weight 30 g ± 0.3 mg	YSS43	
Temperature adjustment set	YTM01MA	
Standard Operating Procedure (SOP)	YSL02MA	

Declaration of Conformity





Sartorius Weighing Technology GmbH Weender Landstrasse 94 – 108 D-37075 Goettingen, Germany

erklärt, dass das Betriebsmittel declares that the equipment

Geräteart: Device type: Feuchtebestimmer Moisture analyzer

Baureihe / Type series:

MA35M-..., MA100.-..., MA150.-..., LMA200PM-...

in der von uns in Verkehr gebrachten Ausführung mit den grundlegenden Anforderungen der folgenden Europäischen Richtlinien übereinstimmt: in the form as delivered complies with the basic requirements of the following European Directives:

Richtlinie 2004/108/EG Directive 2004/108/EC Elektromagnetische Verträglichkeit Electromagnetic compatibility

Richtlinie 2006/95/EG

Elektrische Betriebsmittel zur Verwendung innerhalb bestimmter

Spannungsgrenzen

Directive 2006/95/FC

Electrical equipment designed for use within certain voltage limits

Das Gerät erfüllt die anwendbaren Anforderungen folgender harmonisierten Europäischen Normen. The apparatus meets the applicable requirements of the harmonized European Standards listed below.

1. Richtlinie 2004/108/EG / Directive 2004/108/EC

EN 61326-1:2006 Elektrische Mess-, Steuer-, Regel- und Laborgeräte - EMV-

Anforderungen - Teil 1: Allgemeine Anforderungen (IEC 61326-1:2005) Electrical equipment for measurement, control and laboratory use - EMC requirements - Part 1: General requirements (IEC 61326-1:2005)

2. Richtlinie 2006/95/EG / Directive 2006/95/EC

EN 61010-1:2001

Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte – Teil 1: Allgemeine Anforderungen (IEC 61010-1:2001)
Safety requirements for electrical equipment for measurement, control, and laboratory use – Fart 1: General requirements (IEC 61010-1:2001)

Jahr der Anbringung der CE-Kennzeichnung / Year of attachment of CE marking: 11

Sartorius Weighing Technology GmbH Goettingen, 2011-11-03

associated product documentation must be observed.

Dr. Reinhard Baumfall Vice President R&D Dr. Dieter Klausgrete

Leitung International Certification Management Head of International Certification Management

Diese Erklärung bescheinigt die Übereinstimmung mit den genannten EG-Richtlinien, ist jedoch keine Zusicherung von Eigenschaften. Bei einer mit uns nicht abgestimmten Anderung des Produktes verliert diese Erklärung ihre Gültigkeit. Die Sicherheitshinweise der zugehörigen Produktdokumentation sind zu beachten. This decharation certifies conformity with the above mentioned EC Directives, but does not guarantee product attributes. Unauthorised product modifications make this declaration invalid. The safety information in the

SWT11CE017

65711-000-58

SOP-3.RD-045-fo2

Sartorius Weighing Technology GmbH Weender Landstrasse 94-108 37075 Goettingen, Germany

Phone +49.551.308.0 Fax +49.551.308.3289 www.sartorius.com

Copyright by Sartorius,
Goettingen, Germany.

No part of this publication may be reprinted or translated in any form or by any means without prior written permission from Sartorius.

All rights reserved by Sartorius in accordance with copyright law.

The information and figures contained in these instructions correspond to the version date specified below. Sartorius reserves the right to make changes to the technology, features, specifications and design of the equipment without notice.

Status: February 2012, Sartorius Weighing Technology GmbH, Goettingen, Germany

Printed in Germany on paper that has been bleached without any use of chlorine W_MA35 · KT
Publication No.: WMA6032-e12024



Operating Instructions

Sartorius Moisture Analyzer

Model MA37 Electronic Moisture Analyzer



Contents

User Information	3
Safety Instructions	4
General View of the Equipment	7
Commissioning	8
Transporting the Analyzer 1	2
Basic Principles	3
Operating the Moisture Analyzer 2	20
Switching the Analyzer On and Off (Standby) 2	0
Setting the Language	1
Operating Concept 2	2
Menu 2	23
Entering Numbers on the Number Pad	4
Entering Text and Characters	4
Scrolling in the Display	:5
System Settings (Setup Menu)	6
Opening the Menu and Changing the Settings 2	6
List of Available Settings	27
Moisture Analysis 3	4
Viewing and Changing Method Parameters 3	4
Performing the Moisture Analysis	6
MA Performance Test 4	-0
Starting the Performance Test 4	0
Performance Test Measurement Not Successfully	
Completed 4	2
Performance Test Successfully Completed 4	3

Calibration and Adjustment4
Calibrating/Adjusting the Heating Module 4
Viewing the Calibration Report
Weighing
SO/GLP-compliant Printout 4
USB Port 5
Communication with Peripheral Devices
Interface Specification
Error Messages 5
Shipping the Analyzer 5
Care and Maintenance
Disposal6
Specifications
Accessories6
Analyzer Dimensions
EU Declaration of Conformity
FCC Supplier's Declaration of Conformity 6
CSA Certificate of Compliance

User Information

Warning/Danger Symbols Used in These Instructions:



These notes identify hazards which have a high probability of resulting in death or serious physical injury if not avoided.



These notes identify hazards that can result in moderate or mild injuries if not avoided.



These notes identify hazards associated with the risk of material damage.

Symbols and Signs

The following symbols and signs are used in this manual:



Useful information and tips



Hot surface: Warning: Risk of severe burns!



Note regarding device operation



When individual buttons are displayed, they should be pressed.

The following symbols are used in these instructions:

- ▶ Indicates a required action
- Describes what happens after you have performed a particular step

Perform steps in the specified order:

- 1. First action
- 2. Second action
- 3.
- Indicates an item in a list

Application Advice/Technical Support

Contact addresses for application advice and our technical support can be found online at: http://www.sartorius.com

Safety Instructions

Guidelines and General Information

- The analyzer complies with EU Directives and standards, among other regulations, for electrical safety and electromagnetic compatibility*. Improper use or handling, however, can result in damage and/or injury. Any improper use or operation of the analyzer that is not consistent with the instructions will result in forfeiture of all claims under the manufacturer's warranty.
- Personnel need to have read and understood these installation instructions, including the safety instructions.
- In the event of use in systems and ambient conditions which have greater safety requirements, you must observe the requirements and provisions applicable in your country.
- Always keep the equipment and analyzer freely accessible.
 Any improper installation of the analyzer that is not consistent with the instructions will result in forfeiture of all claims under the manufacturer's warranty.

* = see "Specifications"



Danger of Explosion!

The analyzer must not be operated in potentially explosive atmospheres. Materials liable to catch fire or explode may not be used as samples for moisture analysis.



Before initial startup, ensure that the voltage rating printed on the manufacturer's ID label of the analyzer matches the voltage of the local AC power.

Installation Instructions



Danger of severe personal injury or property damage due to faulty analyzer components! Do not operate the analyzer if the housing or power supply cable, including any connectors, is damaged. Immediately disconnect a damaged analyzer from the power by pulling the plug.



Danger of Electric Shock!

The analyzer has a power supply cable with a protective grounding conductor. Only standard-compliant extension cords with protective grounding conductors are permitted for use with the analyzer.



Do not expose the analyzer, its power supply cable, or accessories supplied by Sartorius to extreme temperatures, aggressive chemical vapors, moisture, shock, vibrations, or strong electromagnetic fields.

Observe the conditions of operation described in the Specifications.



The operator shall be solely responsible for any modifications to the equipment and for connecting any cables or equipment not supplied by Sartorius! Information on operational quality is available upon request from Sartorius. Only use original Sartorius accessories!



Note the IP protection class of the analyzer! Do not allow liquid penetration. The protection class specifies the suitability of equipment for various environmental conditions (moisture, foreign bodies).



Before cleaning the analyzer: Unplug the power supply cable from the socket.



Position the power cable so that it cannot touch the hot surfaces of the analyzer and is not a trip hazard. Disconnecting the grounding conductor is prohibited.

The device may only be opened by specialized personnel trained by Sartorius.

Danger due to Fire or Explosion!



- Flammable or explosive substances
- Substances containing solvents
- Substances that release flammable or explosive gases or vapors during the drying process: When working with these types of samples, use a drying temperature that is low enough to prevent a fire or explosion from occurring.
- If in doubt, carry out a careful risk analysis.
- Wear safety glasses.
- Always work with small sample quantities.

Never leave the analyzer unattended in these cases.



No modifications to the analyzer are permitted.

Symbols Used on the Device



When setting up the moisture analyzer, leave enough space to prevent heat from building up and to keep the analyzer from overheating:

- 1 m above the analyzer
- 20 cm around the analyzer

The vent above the sample must not be covered or modified in any other way. During operation do not open the hood, because the heating unit may be very hot.

Do not put any flammable substances on, under, or near the moisture analyzer because the area around the heating unit will heat up.

Be careful when removing the sample: The sample itself, the heating unit, and the sample pans may still be extremely hot.

Observe the additional safety and danger information in the following chapters.

Personal Protective Equipment

When operating the analyzer, suitable protective equipment must be worn in order to minimize dangers to health.

- During work, always wear the protective equipment needed for the task at hand.
- Follow any instructions posted in the work area pertaining to personal protective equipment.

Wear the following personal protective gear during all work:



Protective Clothing

Wear a laboratory coat. This lab coat protects the user from hazards due to the dangerous substances or is prescribed for your chosen process.



Safety Glasses

Wear safety glasses to protect yourself from liquid spray and splashes and substances escaping under high pressure.



Safety Gloves

Wear suitable safety gloves when handling chemicals or hazardous substances. Check that the gloves are not worn and do not have any holes or tears before putting them on.

Intended Use


The moisture analyzer can be used for quick and reliable determination of the moisture content of materials of liquid, pasty, and solid substances using the thermogravimetric method. Only use the analyzer for this purpose. Any other use outside the limits of the technical specifications is not permitted.

Moisture analysis applications must be optimized by the user in accordance with local regulations.

Appropriate containers must be used for each type of sample material.

All other applications are not considered the intended use. If the analyzer is not used properly, this may adversely affect the safety features of the analyzer.

General View of the Equipment

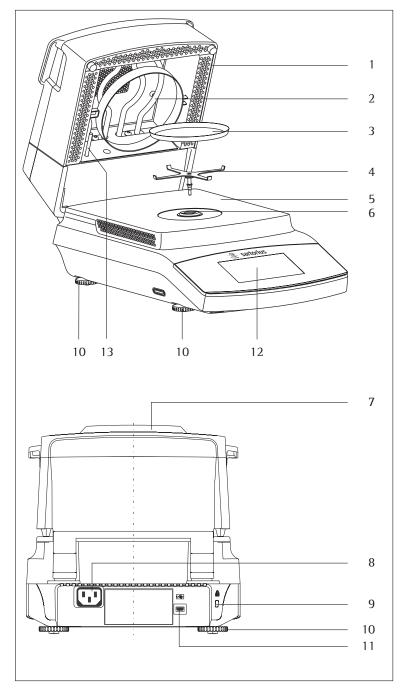

Pos.	Name and Function
1	Heating module
2	Heating element
3	Disposable sample pan
4	Pan support
5	Sample chamber base plate
6	Locking socket (bayonet)
7	Status light
8	Power socket for country-specific power cable
9	Fastening point for an optional Kensington key lock
10	Leveling feet
11	USB port for mini AB
12	Display and control unit (touch screen)
13	Temperature sensor

Commissioning

Unpacking and Equipment Supplied

- ▶ Open the packaging, making sure to remove all parts carefully.
- ▶ After unpacking the analyzer, check it immediately for any external damage.
- If you detect any damage, proceed as directed in "Care and Maintenance."
- Save the box and all parts of the packaging for any future transport.
 During shipment, please do not leave cables plugged in!

The following parts are included in the equipment supplied:

- Moisture analyzer
- Country-specific power cable
- Pan support
- Protective cover for the control panel
- 80 disposable aluminum sample pans
- 40 glass fiber filters (hard quality)
- Operating Instructions

Choosing a Location

► Select the proper setup location:

An optimal location guarantees accuracy and reliability. Ensure that the following ambient conditions are met:


- Set up the analyzer on a stable, even surface that is not exposed to vibrations (e.g., weighing stone).
- Maintain free access to the analyzer at all times.
- Make sure to choose a place where excessive heat cannot build up.
- Leave enough space between it and materials that are affected by heat.

Choose a location that is not subject to the following negative influences:

- Heat (heater or direct sunlight)
- Drafts from open windows, AC systems, and doors
- Extreme vibrations during measurement
- Heavy traffic areas (personnel)
- Extreme humidity
- Electromagnetic fields


Acclimatization

Condensation from humidity can form on the surfaces of a cold device when it is brought into a warm area. You should therefore let a device that has been disconnected from its power source acclimatize for approximately 2 hours before reconnecting it to the power.




Setting Up the Analyzer

- ► Assemble the parts in the following order:
- Pan support
- Disposable sample pan
- The in-use dust cover over the control panel is put into place at the factory.




Compensating for Unevenness of Setup Surface

► Twist the leveling feet until any slight unevenness in the setup surface is rectified and the analyzer is stable.



Anti-theft Locking Device

- To protect against theft, the analyzer has a fastening point for a security lock if required.
- A Kensington key lock can be installed at the fastening point on the back of the analyzer if required.




Opening and Closing the Sample Chamber

▶ Open or close the sample chamber by hand. Always open the heating module fully.

Power Connection (Power Supply)



- Using the wrong power plug adapters may cause fatal electric shock and damage the equipment.
- Never plug the power cable into the socket when it is disconnected from the analyzer (danger of electrical shock).
- Only connect the analyzer to an AC socket with a protective grounding conductor.
- Only standard-compliant extension cords with protective grounding conductors are permitted for use with the analyzer.
- Intentionally disconnecting the analyzer from the protective grounding conductor is not permitted.



- Check the plug design of the power cable. If the plug design of the power cable does not comply with your country's standard, please inform the nearest Sartorius representative or your dealer. The power must be connected in accordance with the regulations applicable in your country. In order to connect the equipment to the power supply (protection class 1), use a correctly installed wall outlet with a protective grounding conductor (PE) and a fuse of a maximum 16 A. The power plug or another suitable disconnecting device for the power must be easily accessible so that the analyzer can be disconnected from the AC power supply in the event of an emergency.
- Connect the analyzer to the AC power.
- ▶ Position the cable so that it cannot be damaged or hinder the measurement process.

Safety Precautions

If you use an electrical outlet that does not have a protective grounding conductor, ensure that an equivalent protective conductor is installed by a certified electrician (as specified in the applicable regulations for installation in your country). The protective effect must not be negated by using an extension cord without a protective grounding conductor.

Power Cable Versions

Region/Country
Europe/EU (except the UK, Denmark, Italy, and Switzerland)
USA, Canada, and Japan
South Africa
Australia, New Zealand
United Kingdom
Brazil
India
Israel
Italy
Argentina
China
Switzerland
Denmark



Warm-up Time

To return precise results, the analyzer must warm up for at least 30 minutes after initial connection to the power supply.


Only then will the device have reached the required operating temperature.

Transporting the Analyzer

Moving the Analyzer in the Lab



Avoid shocks and vibrations.



Never lift and carry the analyzer by its heating module.



► Hold the analyzer under the housing, lift it up carefully, and carry it to its new location.

Basic Principles

Purpose

The moisture analyzer can be used for quick and reliable determination of the moisture content of materials of liquid, pasty, and solid substances using the thermogravimetric method.

Material

The moisture of a material is often mistakenly equated to its water content. In fact, the moisture of a material includes all of the volatile components which are emitted when the sample is heated, irrespective of the type of material. Among such volatile substances are:

- Water
- Fats
- Oils
- Alcohols
- Organic solvents
- Flavorings
- Volatile components, products of decomposition (when a sample is overheated)

There are many methods for determining the moisture content of a substance. Basically, these methods can be divided into two categories:


When absolute methods are used, the moisture content is directly determined (for example, as a weight loss registered during the drying routine). These methods include oven drying, infrared drying, and microwave drying. All three of these methods are thermogravimetric.


When deductive methods are used, the moisture content is indirectly determined. A physical property related to the moisture in the substance is measured (e.g., conductivity). These methods include capacitive and spectroscopic approaches.

Thermogravimetry is the process of determining the loss of mass that occurs when a substance is heated. In this process, the sample is weighed before and after being heated, and the difference between the two weights is calculated.

In a conventional drying oven, circulating hot air warms the sample from the outside to the inside. Efficiency is lost during drying because as the moisture evaporates, it cools the sample surface.

By contrast, infrared rays (IR rays) penetrate the substance. The majority of the rays reach the interior of a sample, and then directly heat the sample.

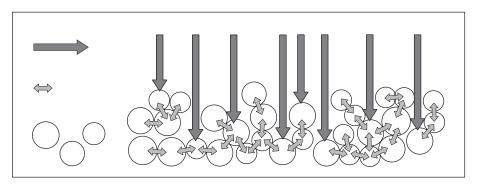




The proportion of the IR rays which does not heat the sample is either reflected on the surface of the sample or penetrates the sample unimpeded.

The color and surface properties of the sample significantly influence how effective the heating process is. For example, dark substances absorb IR rays better than bright substances.

How the rays penetrate the sample depends on the permeability of the sample. If the degree of light-transmitting capacity is low, the rays can penetrate only the uppermost layers of the sample. The heat conductivity of the sample dictates the degree to which the heat can be transmitted to the underlying layers. The higher the conductivity, the faster and more uniformly the substance is heated.

The substance should be applied to the sample pan in a thin, even layer. A height of approximately 2–5 mm for 5–15 g substance weight has proved to be ideal. Otherwise, the sample will not be dried completely or the analysis time will be unnecessarily extended, a crust/skin will form on the surface of the sample or the sample will scorch, and the analysis results obtained will not be reproducible (and hence cannot be used).

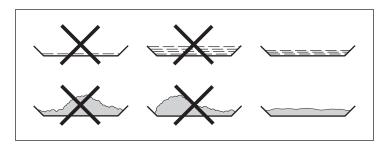

While preparing substances for measurement, no processes may be used that generate heat. The heat generated may result in a loss of moisture prior to the measurement.

Perform initial analysis of a new substance to test how the IR rays are absorbed by the sample and converted into heat. A printout of the intermediate values of the drying process provides information on this at an early stage.

Since introducing IR rays produces intensive energy input in the sample, the temperature setting selected for infrared drying is usually lower than the temperature setting used when working with a drying oven.

In many cases, the fully automatic switch-off mode will meet your requirements. If the final result is higher or lower than expected, try varying the temperature setting before resorting to a different switch-off criterion.

When analyzing the samples that lose their moisture only very slowly or when operating a cold moisture analyzer, the fully automatic mode may end the drying routine too early since no analyzable progress in the drying routine can be detected. In this case, preheat the moisture analyzer for two to three minutes before starting the drying routine, or select a different switch-off criterion.



The Application Guide for the Sartorius Moisture Analyzer provides you with important information on the use of your moisture analyzer.

Preparation

Before drying a sample, you must carry out the following preparations:

- Adjust against the existing measurement system
- Prepare the sample
- Set the drying program parameters

Adjusting against an Existing Measurement System

A moisture analysis method often replaces another drying method (such as oven drying method) because it is simple to use and requires shorter analysis time. In this case, you should adapt this method to that of the moisture analyzer in order to obtain values comparable to those yielded by your standard reference method.

Perform parallel measurements:

- ► Take a fresh sample and divide it in half
- ▶ Determine the moisture content of the first half using your standard method of analysis
- ▶ Determine the moisture content of the second half using the following settings:
 - Fully automatic mode for the switch-off criterion
 - Lower temperature settings than for the oven drying method
 - Temperature setting for organic substances: 100–130 °C
 - Temperature setting for inorganic substances: 180-200 °C

If the result of the second analysis does not correspond to that of the first:

- 1. First, repeat the analysis using a different temperature setting
- 2. Then use the semi-automatic mode for the switch-off criterion (for example, with a different loss rate per 24 s)

Change the switch-off criterion if required:

- Increase end-point recognition: Set the parameter to 2 mg/24 s or 1 mg/24 s
- Decrease end-point recognition: Set the parameter to 10 mg/24 s or 20 mg/24 s

Preparing the Sample

Select a sample:

- ▶ Select a representative part of the whole substance as a sample.
 - Choose a representative number of individual samples for quality control
 - Choose enough samples to indicate a trend for in-process control
- ▶ If required, homogenize the product before a sample is taken by:
 - Mixing or stirring
 - Taking several samples from different areas of the product
 - Taking several samples at defined intervals
- ➤ Take only one sample at a time for a given analysis and prepare it as quickly as possible. In this way, it will not lose or gain moisture as a result of the ambient conditions.
- ▶ If several samples need to be taken simultaneously, the samples must be sealed in airtight containers to ensure that the storage conditions do not alter the state or condition of the samples:
- Warm or highly volatile substances lose their moisture very quickly.
- If you store the samples in a container, the moisture can condense on the walls of the container.
- If the container is too big and not filled completely, the sample can exchange its moisture with the air remaining in the container.

▶ Mix the condensed moisture back in with a sample if necessary.

Prepare the sample:

- ► When crushing a sample, avoid any contact with heat. Heat results in moisture loss.
- ► Crush the sample using:
 - Pestle
 - Lab mill

If the sample is liquid containing solids, use one of the following tools:


- Glass stirrer
- Spoon
- Magnetic stirrer
- ▶ Use an appropriate tool for grinding the sample.

Use a disposable sample pan:

- ► Use only Sartorius disposable sample pans (inner diameter of 90 mm). Reusing sample pans leads to poor repeatability of results:
 - After cleaning, sample residues can still remain on the pan.
 - Residues from cleaning agents can evaporate during the next moisture analysis.
 - Scratches and grooves made during cleaning result in damage that forms points of attack for hot, rising air produced during the drying process (more pronounced buoyancy).

Distribute the sample on the sample pan:

- ▶ Distribute the sample on the sample pan in a thin, even layer (height: 2 to 5 mm, weight: 5 to 15 g); otherwise:
 - A sample applied unevenly will result in a nonuniform distribution of heat
 - The sample will not be dried completely
 - The analysis time will be unnecessarily extended
 - The sample will burn or a crust/skin will form on its surface as a result of a very thick layer
 - The crust makes it difficult or impossible for moisture to escape from the sample during the drying process
 - An uncertain and unknown quantity of moisture will remain in the sample

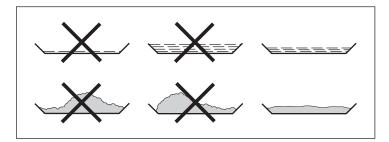

- ▶ Apply liquid samples, pasty samples, or samples that can melt to a glass-fiber filter (order no. 6906940); this provides the following benefits:
 - Uniform distribution due to the capillary effect
 - Liquids are prevented from beading together and forming drops
 - With larger surfaces, the moisture can evaporate faster
 - Colorless/transparent samples do not reflect
 - Considerably more convenient than the "sea-sand method"

When drying samples containing sugar, a crust or skin can form and seal the surface. A glass-fiber filter is particularly useful in such cases. The moisture can evaporate downwards through the surface of the filter. Crust/skin formation can be prevented or limited by placing the glass-fiber filter on top of the sample.

- ► Cover solid, heat-sensitive samples with a glass-fiber filter (order no. 6906940); this provides the following benefits:
 - Gentle heating, because the sample surface is shielded from excessive heat
 - Higher temperature setting can be selected
 - Uniformity of the sample surface
 - Fast evaporation of the moisture
 - Excellent repeatability for samples containing fat


Heating Programs


Three heating programs are available for performing moisture analysis of a substance:

- Standard drying
- Gentle drying
- MA35 mode

Standard drying:

For standard drying, you need to enter the final temperature. The final temperature is reached using an overshoot if necessary. The maximum set temperature is 200 °C.





Gentle drying:

For delicate drying, you need to enter the final temperature.

The maximum set temperature is 200 °C. The target temperature is reached more slowly and the measurement time is extended, but an overshoot is avoided. Gentle drying is recommended for sensitive samples.

MA35 mode:

The moisture analyzer heats as in the standard mode, but converts to values on the temperature scale corresponding to those in the MA35 (old adjustment disk technology; $40-200~^{\circ}\text{C} \rightarrow 40-160~^{\circ}\text{C}$). This mode is active only for moisture analysis (before, during and after drying), but not during heat adjustment or heating tests.

Standby Temperature

Temperature set to defined value when the sample chamber is closed. Heating only occurs when the analyzer is in a measurement cycle. The standby temperature is not the same as the measurement temperature.

The "Timeout Standby Temp." can be set to 1 to 24 hours and is preset to 2 hours. To change the setting, see chapter "System Settings (Setup Menu)."

Initial Weight

The target weight and the associated tolerance range can be entered by the user as mandatory or just as a weighing guide. The tolerance range can be freely selected, e.g., \pm 0.5 g.

Print Lines

When print lines are activated (1 or 2 lines with 20 characters each), additional information about the method, entered by the user, appears on the report and printout.

Filters

The user has the option of selecting between 0, 1, or 2 filters. During taring a message appears indicating that the configured number of filters must be placed with the sample pan for taring.

Target Value

The user can enter a target value with a tolerance range. During analysis a progress bar appears, indicating the progress of the measurement. At the end of the analysis, you can see whether the value is within the tolerance range.

Starting the Analysis

- After closing the hood:

If the initial weight condition is met, the analyzer prompts you to close the hood. The start weight is applied as soon as the sample chamber is closed and the measured value is stable.

End of Analysis

Fully automatic

The analysis ends as soon as the weight loss per 24 s is below an automatically detected threshold.



The analysis ends as soon as the weight loss per the set interval is lower than a user-defined threshold (set in milligrams).

The weight loss is entered by the user.

- Semi-automatic, percentage

The analysis ends as soon as the weight loss in percent is lower than a user-defined threshold (set in percent).


The percentage is entered by the user.

– Time

The analysis ends as soon as the specified time has elapsed.


- Manual

Switch off using the END key. The maximum analysis duration is 24 hours.



Operating the Moisture Analyzer


Switching the Analyzer On and Off (Standby)



- > The main screen appears after the moisture analyzer has been switched on.
 - The default language for the display text is English.You can change the language (see "Setting the Language" on page 21).



► To switch the moisture analyzer to standby, select the menu key at the bottom left of the main screen on the display.



➤ The menu is displayed.



- ► Select the 🖒 button in the menu.
- ➤ The moisture analyzer switches to standby mode.



► To switch the moisture analyzer on again: Select 🖒 on the display. The moisture analyzer starts in the method most recently used before the analyzer was last switched off.

Setting the Language

The default language for the display text is English. To change the language, proceed as follows:




▶ Select the menu key at the bottom left of the main screen on the display.



➤ The menu is displayed.



▶ Select the 🔑 (Setup) button in the menu.



- > The **Settings** window appears.
- ► Select **Language** or the top entry in the list.



- ➤ The Language settings window appears.
- ▶ Select the desired language, such as **Deutsch** (German).
- ▶ Select ✓ to confirm.
- > The display changes directly to the desired language.
- ► Select **<** to return to the menu.

Operating Concept


This section explains the operating options available to you so that you can familiarize yourself with the moisture analyzer.

Operating and Display Elements



Sharp or Pointed Objects (such as Ballpoint Pens) Can Damage the Device.

- The touchscreen should only be operated by lightly pressing it using the tips of your fingers. You can also operate the touch screen when wearing lab gloves.

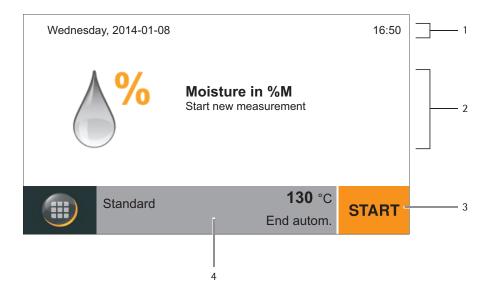


- 1 Current date and time
- 2 Selected result display for the method
- 3 Operate method, such as start moisture analysis
- 4 View settings for the selected method

Menu


All settings for the moisture analyzer can be accessed via the menu.



- ▶ To access the menu, select the menu key at the bottom left of the display.
- ▶ The menu opens.

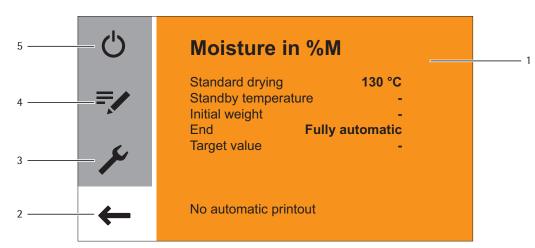

- 1 Method with current parameters
- 2 Back to the main screen
- 3 Setup menu: Open system settings (see page 26)
- 4 Change method parameters
- 5 Switch moisture analyzer to standby mode




Entering Numbers on the Number Pad

You can enter numeric values in the method parameters or system settings (such as the temperature setting for a heating program). A number pad appears on the display, which is always used in the same way.

- ▶ To enter numbers, select the desired numbers one after the other.
- ▶ The entered numbers appear at the top of the display.
- ► To correct the last entered number, select ←.
- ▶ The number is deleted. Then enter the correct number.
- ► To clear the entire entered value, select **C**.
- ightharpoonup To confirm the entry, select \checkmark .

Entering Text and Characters



A keyboard will appear when you have to enter text and characters.

➤ Select the individual characters one after the other. The entered text appears at the top of the display. If you hold down a character for longer, the special versions of that character (umlauts, accent marks) and special characters appear.



- ▶ Use the Shift key to switch the keyboard display between uppercase and lowercase letters.
- 123
- ▶ Use the 123 key to switch the keyboard display from letters to numbers.
- ABC
- ▶ Use the ABC key to switch the keyboard display from numbers to letters.



▶ Use the back arrow key to delete the last character.




► The ✓ key ends the process and saves character input.

Scrolling in the Display

If more than one entry is available, you can scroll up and down through the display to select the desired entry.

- ▶ To scroll, place your finger on the display and drag it slowly either up or down.
- ➤ The entries on the display move in the corresponding direction. While you are scrolling, a gray scroll bar appears on the right of the display, indicating where you are in the list of options.



<

Settings
Date and time

Printout

Device information

Calibration/Adjustment

► Tap the desired entry to select it.

System Settings (Setup Menu)

The **Settings** (Setup) menu contains all basic settings for the moisture analyzer.

Opening the Menu and Changing the Settings




▶ Select the menu key on the main screen.




The menu is displayed.



Select the \(\sum_{\color \text{(Setup)}} \) key in the menu.



> The **Settings** (Setup) menu appears.



- ► To scroll, place your finger on the display and drag it slowly either up or down.
- ➤ The entries on the display move in the corresponding direction. While you are scrolling, a gray scroll bar appears on the right of the display, indicating where you are in the list of options.
- ► Select a setting and make the desired change. Information about the available settings can be found from page 27.
- ▶ Select ✓ to confirm your changes.
- ► Select < to return to the menu. The changed settings are active when you reach the first level of the menu again.

List of Available Settings

This section contains information about all of the basic settings on the moisture analyzer, which can be defined in the **Settings** menu.

Language

The language of the display text can be set here. English is set as the default language on the moisture analyzer (see "Setting the Language" on page 21).

The following languages are available. Each language option is presented in that particular language.

- English
- German
- French
- Spanish
- Italian
- Japanese
- Russian
- Chinese
- Polish
- Portuguese
- Turkish

Date and Time

The date, time, and display format can be set here.

Under Date:

 \blacktriangleright To set the date, select \cdots , enter the current date and confirm with \checkmark .

Under Date format:

- Select how the date is displayed and printed out.
 - DD-MMM-YYYY:

The date is displayed in the order of day, month and then year.

- MMM-DD-YYYY:

The date is displayed in the order of month, day and then year.

- YYYY-MM-DD (ISO):

The date is displayed in the order of year, month and then day. (The time is always displayed in 24-hour format with this setting.)

Under Time:

ightharpoonup To set the time, select \cdots , enter the current time and confirm with \checkmark .

Under **Time format**:


- ▶ Select how the time is displayed and printed out.
 - 24h

The time is displayed in 24-hour format. (This is the only available setting when the date is set to ISO format.)

- 12h (AM/PM)

The time is displayed in 12-hour format. The hours before noon are displayed with **AM** and the hours after noon are displayed with **PM**.





Device information

/

Manufacturer: Model: Serial number: Version BAC: Version APC: Version MCU:

<

Sartorius MA37 0000021087 00-53-01.01.00 01-80-01.09.01 07-40-05.00.00

Calibration/Adjustment

MA performance test
Weighing system adjustment
Cal./Adj. the Heating Module
Calibration report

Device Information

The manufacturer, model, serial number, and software version of the moisture analyzer are displayed here.

Calibration/Adjustment

The settings for calibration and adjustment of the moisture analyzer can be defined here.

Under MA Performance Test:

Test functions for different temperature ranges are available here. You can only use these functions with the ReproEasy pad (accessory).

Under Weighing system adjustment:


- Select the option of your choice.
 - CAL-Extern: Carry out calibration with an external calibration weight (see section "Calibrating the Weighing System" in chapter "Calibration and Adjustment").
 - Weighing only: Use the weighing function to use the moisture analyzer as a simple lab balance (see section "Weighing" in chapter "Calibration/ Adjustment").

Under Heater module cal./adj.:

You can calibrate and adjust the heating module here in connection with the YTM15MA heating adjustment set. (see section "Calibrating/Adjusting the Heating Module" in chapter "Calibration and Adjustment").

Under Calibration report:

You can view the current calibration reports on the MA performance tests, weighing system adjustment, and heating module calibration and adjustment. Up to 99 logs per day are saved. Calibration reports older than 30 days are deleted. Only the current calibration report is saved for each calibration or adjustment of the heater.



Printout

You can configure the settings for printing and data output here. Some of the settings depend on the USB port configuration (see "USB Port" on page 31). Under **Printout measurement**:

- ▶ Select the settings for printing out the results on the connected lab printer.
 - **Printout measurement:** The printout can be activated and deactivated during the measurement here.
 - **Interim results**: If the printout is activated, you can also activate the output of intermediate values during the measurement here.
 - Interval [sec]: Enter the desired interval in seconds for the output of the intermediate results.

Under Printout and Report Format:

- Configure all settings for the output format.
 - Result only: Only the result of the moisture analysis is output.
 - With GLP and method parameters: The GLP data and parameters used for the moisture analysis are also output.



Signals

The key tones, acoustic signals, and status light can be switched on and off here.

The following settings are available for each signal:

- On: The signal is activated.
- Off: The signal is deactivated.



<

Signals

Touch signals

Acoustic signal


Status light

Display Brightness

The brightness of the display can be set here.

The following brightness levels are available:

- Bright
- Medium
- **Eco mode**: Energy-saving mode (factory setting): The brightness is reduced after 2 min. of inactivity. To reactivate the normal brightness: Touch the screen or open the heating module. During measurement and during the results display, eco mode is deactivated.



Identifiers

The identifiers for the printout can be defined here.

- The **Device ID** identifier is entered here once. The device ID can be a maximum of 14 characters long.
- The Batch ID and Sample ID functions can be activated here. The user must then enter the batch and sample IDs before each measurement routine. Batch and sample IDs cannot exceed 20 characters.

Under **Device ID**:

The device identifier (ID) is printed in the header of the GLP printout.

To set the device ID, select **Device ID**, enter the desired device ID and confirm with ✓.

Under Batch ID function:

The batch ID (L ID) is queried once at the beginning of the measurement routine.

▶ If you wish to print the batch ID, activate this option.

Under Sample ID function:

The sample ID (S ID) is queried once at the beginning of the measurement routine.


▶ If you wish to print the sample ID, activate this option.





To enter and delete numbers and text, e.g., for the sample ID, see "Entering Text and Numbers" on page 24.

Timeout Standby Temp.

The timeout for the standby temperature can be set here.








USB Port

The settings for the data transfer to a peripheral device (such as a PC or printer) can be defined here.

Depending on the cable and peripheral device connected to the moisture analyzer, various options are available in the menu. The moisture analyzer automatically detects the type of connection.

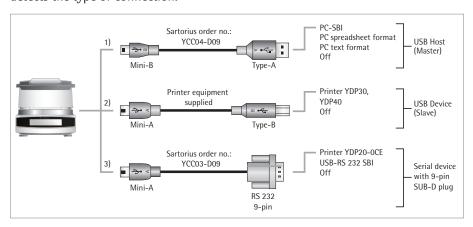


There are several ways to connect the device via USB:

1) Connection to a PC via USB cable (Mini-B to USB A)

Under **Device/Protocol**:

- Select the data format for the transfer to the PC.
 - PC SBI: Driver for PC required (CDC Virtual Com Port). The data is sent via SBI protocol using a virtual serial interface. Further information can be found in chapter "USB Port: Direct Transfer of Data (PC)."
 - PC spreadsheet format: The analyzer transmits the data via keyboard command (keyboard emulation) to the currently opened application on the PC in spreadsheet format.
 - PC text format: The analyzer transmits the data via keyboard command (keyboard emulation) to the currently opened application on the PC in text format.
 - Off: Data transmission is deactivated.



Under **Decimal separator** (also available when "PC spreadsheet format" has been selected):

- Decimal point (factory setting): The number value is transmitted with a decimal point to the PC program (example: 99.963 g).
- Decimal comma: The value is transmitted with a decimal comma to the PC program (example: 99,963 g).

Under **Keyboard emulation** (also available when "PC spreadsheet format" or "PC text format" has been selected):

- Universal (Num Lock On) (factory setting): Data is sent as special keyboard characters in ASCII format (ALT + number pad).
 - Requirement: Numbers lock must be turned on on the PC keyboard.
- English (USA): Data is sent according to a keyboard set to English (USA).
 Requirement: For PC applications, such as MS Excel, the keyboard must be set to English (USA).



Further information can be found in chapter "USB Port."

2) Connection to Sartorius Lab Printer via the Supplied Printer Cable

Under **Device/Protocol**:

- Select the desired setting for the connection to the printer.
 - YDP30/YDP40: The connected printer is detected automatically and the connection is established.
 - Off: The connection to the printer is deactivated.

3) Connection to a Serial Printer or Another External Serial Device via a 9-pin Serial Interface (USB Mini-A to RS-232)

Under **Device/Protocol**:

- Select the desired setting for the connection to the device.
 - Printer YDP20-0CE
 - USB-RS-232 SBI
 - **Off**: The connection is deactivated.


Check the settings on the **Printer YDP20-0CE**:

- Set the printer to factory settings:
 - 1200 baud, 7 bits, ODD parity, 1 stopbit, CTS/RTS handshake

Under RS-232 Configuration:

This option can be selected if under **Device/Protocol** the setting **USB-RS-232 SBI** has been selected.

- ► Select the desired setting for the RS-232 interface.
 - **Baudrate**: 600 to 19,200 (factory setting: 9600)
 - Databits: 7 bits or 8 bits (factory setting: 8 bits)
 - Parity: odd, even, or none (factory setting: odd)
 - Stopbits: 1 bit or 2 bits (factory setting: 1 bit)
 - Handshake: software (XON, XOFF), hardware (CTS, RTS), or off [factory setting: hardware (CTS, RTS)]



Service Mode/Service Access

This function is used by the Sartorius Service Center and can only be accessed by authorized service technicians.

Reset

All settings can be reset to the factory settings here. Any user-defined methods, results, and calibration reports are retained.

When the security prompt appears, select Yes, reset and confirm with ✓. The moisture analyzer is reset and restarts.

Moisture Analysis

Purpose:

The moisture analyzer can be used to determine the moisture content of liquid, pasty, or solid samples.

Accessories:

Depending on the consistency of the sample, one or two filters are recommended in order to distribute the sample optimally in the sample pan.

- Liquid sample: Tare one filter with the sample pan, then distribute the sample drop by drop onto the filter.
- Pasty sample: Tare two filters with the sample pan, then place the sample between the two filters and press together evenly.
- Solid sample: Distribute the granulated sample evenly onto the sample pan
 without a filter. Use one or two filters for solid samples that liquefy at high
 temperatures or contain fat or sugar, in order to prevent crusting.



Danger of Poisoning or Caustic Burns!

Substances that contain poisonous or caustic ingredients may produce poisonous gases when dried, which can cause irritation (to the eyes, skin, or airways) or nausea and lead to serious injury or death.


- These samples must only be dried in a laboratory hood.



Corrosion Due to Aggressive Vapors!

Substances that emit aggressive vapors when heated may cause condensation to form on cooler housing parts and lead to corrosion.

- Use small sample quantities of these substances.



Viewing and Changing Method Parameters

Before starting the moisture analysis, you can view the current parameters and change them if necessary.

 A method configuration for moisture analysis is preset. You can change and save the parameters to suit your requirements.

The most important parameters (method name, temperature, switch-off criterion) are displayed.

- ► To check additional parameters, select the gray button at the bottom of the main screen on the display.
- A summary of the current parameters is displayed.

If a lab printer is connected, you can print out the method parameters:

- Select the print symbol.
- ➤ The parameters are printed out.
- Select ✓ to close the display.



► To change the parameters, select the menu key at the bottom left of the main screen on the display.







The menu is displayed.



▶ Select the button in the menu.



> The current method parameters are displayed.




Select the parameter you wish to change, such as "Heating program."




- ► Set the parameters to suit your requirements.

 Select · · · if necessary and enter the desired values (see "Entering Numbers on the Number Pad" in chapter "Operating the Moisture Analyzer").
- ► Select ✓ to confirm.



- ▶ Scroll through the list if necessary and change further parameters.
- ▶ When you are finished making changes, select **<**.



- ➤ The changed method parameters are displayed.
- Select the desired option:
 - Make further changes: Select X. This takes you back to the list of parameters.
 - Reject changes: Select NO.
 - Save changes: Select YES.
- ➤ The menu is displayed.
- ► To return to the main screen, select ←.

Wednesday, 2014-01-08 16:50 Moisture in %M Start new measurement Standard 130 °C Fully automatic

Performing the Moisture Analysis

When all parameters have been set to suit your requirements, you can start the moisture analysis.

Observe the following instructions in order to ensure successful measurement:

- Wear gloves for each measurement, so that the liquid in the sample is not influenced by handling.
- Remove the sample directly from the process or keep it in an airtight and watertight container until measurement.
- Ensure that the sample is representative for the product and is homogeneous (shake, stir, or mix before measurement).
- If using a filter or filters, store the filters in airtight and watertight packaging.



► Select **START** on the main screen or open the hood.




If you selected **START** on the main screen:


- Open the hood now.
- ▶ The next step is displayed when the hood is opened.



- ▶ Place an empty sample pan on the analyzer, along with one or two filters if necessary. The number of filters depends on how many filters are set in the parameters for the current method.
- ► Close the hood.
- > The moisture analyzer tares automatically.



Open the hood.



Place the sample on the sample pan or filter(s).



- ▶ If you have activated the "Initial weight" option in the method parameters (setting "On" or "Mandatory"), a target value display appears.
- Add the sample to the sample pan slowly. When the sample quantity reaches the preset range, the target value display turns green.


If the "Mandatory" setting has been selected, the measurement only starts if the initial weight is within the permissible range.

If the "On" setting has been selected, the measurement also starts if the initial weight is outside of the permissible range.




- ► Close the hood.
- > The moisture analysis starts automatically.

 During the measurement, the process status light on the analyzer flashes, if the light has not been switched off in the menu.



- ➤ The current measurement value and progress are shown on the display during the moisture analysis.
- If a target value is set, the measurement process is displayed as a bar diagram.
 The target value is marked and tolerance limits are displayed.




 If no target value is set, the measurement process is displayed as a curve diagram.

The following information is also shown on the display:

- Information bar at the top right: measurement time expired
- Function bar below: method name, target temperature, switch-off criterion
- ► To cancel the moisture analysis before it is finished: Select X. In the confirmation dialog that follows, select X again.
- ▶ When the moisture analysis is finished, the moisture content of the sample is shown on the display.

The status light on the analyzer flashes three times and then goes out.



- Bar is red: Result is not within the tolerance limits.
- Bar is orange: Measurement was canceled.



- 11:18 min 85.15 %M

 © Measurement completed

 Standard 110 °C End autom. OK New
- If no target value is set, the moisture content is displayed as a curve diagram.
- Select the desired option:
 - To perform another moisture analysis using this method: Select NEW.
 - To view the report and print it out if desired: Select □.
 - To exit the measurement: Select **OK**.

Printing Out the Analysis Report

If a lab printer is connected, you can print out the result of the moisture analysis.



- ▶ Select <a>□.
- ➤ The analysis report is printed out.



The settings for the analysis report can be configured in the system settings [see section "Printout" in chapter "System Settings (Setup Menu)"]. Further information and an example of an analysis report can be found in chapter "ISO/GLP Report."

Removing a Sample



Danger of Burns due to Hot Sample Pan!

The sample and sample pan may be very hot.

- Do not touch the sample pan.
- Use sample forceps (accessory) to remove the sample.



➤ When you have exited the measurement by selecting **OK**, you can remove the sample from the moisture analyzer.

- Open the hood.
- ▶ Remove the sample pan from the moisture analyzer using sample forceps.
- ► Close the hood.
- Allow the sample to cool down and dispose of it properly.


39

MA Performance Test

The performance test can be used to check whether the analyzer has a fault or is ready for operation. During a performance test, both the heating unit and the weighing system are tested at the same time. A ReproEasy pad (accessory) is required to conduct a performance test.

Starting the Performance Test

- Select "MA performance test."
 - ▶ The display switches to a view with three heating temperatures.






Ensure that the analyzer has not been heated for at least one hour before conducting a performance test.



► Select **x** to confirm the message and start the performance test again later.



Select one of the suggested temperatures given for the method you are using.



- Open the hood.
- ➤ The next step is displayed when the hood is opened.




- Place a sample pan on the analyzer.
- Close the hood.
- ➤ The moisture analyzer tares automatically.




Open the hood and remove the sample pan.



- ▶ Open the packaging of the ReproEasy pad (accessory) and remove the pad.
- ► Remove the protective wrapping.



Affix the pad to the center of the sample pan, sticky side down.



▶ Place the sample pan with the "ReproEasy pad" (accessory) reference sample on the pan support.



- Close the hood.
- ➤ The performance test starts automatically. During the performance test, the status light on the analyzer flashes, if the light has not been switched off in the menu.



➤ The display shows the remaining time for the test.

The curve for temperature-related weight loss is analyzed during the test. to determine whether the drying loss per time unit falls within the tolerance range. If it does fall within the tolerance range, the analyzer's function is assured. The measure for this is the calculated MApi value (Moisture Analyzer performance index).

Canceling the Performance Test


- ➤ To cancel the performance test, select X.
- ▶ The message "Measurement canceled" appears.
- ▶ Select ✓ to confirm.
- ➤ The display switches back to the menu.



Performance Test Measurement Not Successfully Completed

If a fault has been detected:

- ➤ The message "Device is not OK." appears.
- ► Select 🖹 to print the performance test result if necessary.
- ▶ Select ✓ to confirm.






Contact the Sartorius Service Center if the message "**Device is not OK.**" appears.

Performance Test Successfully Completed

The analyzer is in working order and displays the message "Device is OK." if the MApi value falls within the following ranges:

Temperature setting	Tolerance range
85	between 9 and 11
125	between 16 and 18
165	between 21 and 25



- ▶ If the test is successful, the message "Device is OK." first appears. Then the analyzer indicates that the sample can be removed.
- ► Select 🖹 to print the performance test result if necessary.



- Select ✓ to confirm.
- > You can remove the sample and return to the menu.

Calibration and Adjustment

Background

During **calibration**, a calibration weight is used to determine how much the displayed value deviates from the actual measurement value. This deviation is compared against a preset target value. The subsequent **adjustment** corrects this deviation or reduces the permissible error limits.

Calibration and adjustment are combined in one process in the moisture analyzer.

When and How Often

The moisture analyzer must be calibrated and adjusted, for example:

- When the ambient conditions have changed (temperature, humidity, or air pressure)
- When the moisture analyzer is set up in a different location or moved in its current location.



An external calibration weight is required for calibration and adjustment (50 g).


Please note the tolerance of the calibration weight being used.

Calibrating the Weighing System

► Make sure that the pan support is empty.




Select the menu key on the main screen.



➤ The menu is displayed.




► Select the 🗲 (Setup) key in the menu.




- > The **Settings** (Setup) menu appears.
- Select Calibration/Adjustment.

- Calibration/Adjustment

 MA performance test
 Weighing system adjustment
 Cal./Adj. the Heating Module
 Calibration report
- Select Weighing system adjustment.
- Select CAL-Extern to calibrate the analyzer using an external calibration weight.
- ➤ The Calibration/Adjustment window appears.
- ▶ Close the hood and select ✓ to confirm.
- ➤ The CAL-Extern window appears.
- Zero the integrated weighing system if necessary.





- A message appears on the display, prompting you to place the calibration weight on the analyzer (50 g).
- Place the calibration weight on the pan support.
- Calibration starts automatically. When calibration is complete, a report appears on the display. The report gives the deviation detected during calibration. You are asked whether the weighing system should be adjusted. After adjustment the report shows the result of the adjustment.
- ► Close the report: Select **x**.
- ➤ The moisture analyzer is now calibrated. If you have also carried out an adjustment after calibration, the moisture analyzer is also now adjusted.

Calibrating/Adjusting the Heating Module

► To calibrate and adjust the heating module, please read the operating instructions for the "YTM15MA heating adjustment set."

<

Calibration/Adjustment

MA performance test
Weighing system adjustment
Cal./Adj. the Heating Module
Calibration report

Calibration Report

MA Performance Test
Weighing system adjustm.
Heater calibration
Heater adjustment
2-point cal. heater

Viewing the Calibration Report

To view the most recent calibration reports: Go to the **Calibration/Adjustment** menu and select **Calibration report**.

You can select recent reports (see following figure) and then sort the calibration reports by date. Up to 99 entries per day are saved. Calibration reports older than 30 days are deleted. Only the current calibration report is saved for each calibration or adjustment of the heater.

➢ "Calibration report" menu.

Example of a Calibration Report:


2016-0	3-29)	12	:02
Sa	rtor	ius		
Mod.			MA3	7-1
SerNo.		0031	710	609
BAC:		00	-53	-01
APC:		01	-80	-01
MCU:		07	-40	-05
2016-0	1-30	1	12	:02
Extern	al c	alib	rat	ion
Start:	man	uall	у	
Set	+	50.0	00	g
Dev	_	0.0	02	g
Extern	ala	djus	tme	n t
Dev		0.0	00	g
Temp	+	23	. 7	' C
Name:				

Weighing


The moisture analyzer also has a simple weighing function which can be opened via the system menu.



► Select the (Setup) key in the menu.



> The **Settings** (Setup) menu appears.



- Go to Calibration/Adjustment and select Weighing system adjustment.
- Select Weighing only.



➤ The weighing screen appears.
You can now use the moisture analyzer as a simple lab balance.



- ► To exit the weighing function, select **END**.
- ► Select < multiple times to return to the menu.

47

1SO/GLP-compliant Printout

Characteristics

You can have the device information, device ID, and the current date printed before (GLP header) and after (GLP footer) the values from the weighing series. The following data is printed:

GLP header:

- Date, time at the start of a weighing series
- Manufacturer
- Model
- Model serial number
- Software version number of the weighing system (BAC)
- Software version number of the display (APC)
- Software version number of the heating module (MUC)
- Device ID with max. 14 characters (if activated under system settings)

GLP footer:

- Field for signature

Configuration

To print out the ISO/GLP report, define the following system settings [see section "Printout" in chapter "System Settings (Setup Menu)"]:

Activate ISO/GLP-compliant printouts: In the Printout menu under Printout and Report Format, activate the With GLP and method parameters option.

Operation

▶ Print out the report after moisture analysis: Select 🖹.

Example of Analysis Report

2016-02-24 10:03 MA37
SerNo. 0000041535
BAC: 00-53 Sartorius APC: 01-80-01 MCU: 07-40-05 Type Standard drying Temperature 130 'C Standby 0 f f Initial weight 0 f f End Fully automatic Result display Moisture in %M Target value 0 f f No. of filters 0 Start time 10:03 Start weight + 4.564 g ${\tt Measurement\ time}$ 00:24 min Result 0.71% M Final weight + 4.531 g Measurement complete Name:


USB Port

Communication with Peripheral Devices

Purpose:

The interface is used to exchange data with connected peripheral devices: Measured values and parameters are sent to a printer or PC. Control commands and data inputs can also be sent to the analyzer from connected devices such as a PC. The USB port can be used to transmit data via the SBI protocol.

The following connections to peripheral devices are possible:

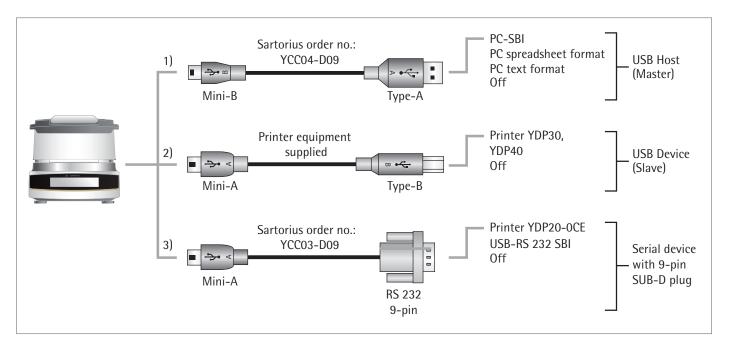

Direct Transfer of Data (PC)


Requirements:

- PC with Windows 7, Windows 8, Vista, Windows XP, or 2000 operating system
- A to Mini-B USB connection cable from PC to moisture analyzer, Sartorius order no. YCC04-D09
- PC with internet connection



The USB driver for the virtual interface is Microsoft®-listed and available online via the Microsoft® Update Service.

PC without internet connection: Please contact your local Sartorius Service Center to load the USB driver.

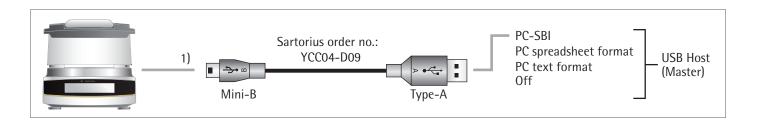


(1) USB Connection as PC Keyboard without Additional Driver via a PC with Table or Spreadsheet Editor (e.g., Microsoft® Office or OpenOffice)

► Connect the moisture analyzer to your PC using the designated USB connection cable.




► To open the system settings of the moisture analyzer, select 🗡 (Setup) in the menu.




➤ To open the **PC spreadsheet format** menu item on the moisture analyzer, go to **USB port** and select **Device/Protocol**.

Setting Options:


- ➤ To change the moisture analyzer to suit your PC settings, define the following system settings [further information can be found in chapter "System Settings (Setup Menu)", USB Port]:
- Choose the character to be used as a decimal point for the spreadsheet calculation.
- Emulation of the PC keyboard for English (USA) instead of Universal (Num Lock on):
- ▶ Once data has been transferred to your PC, the following appears on the PC:
 - When **PC spreadsheet format** is set on the moisture analyzer, e.g., when Microsoft Excel is opened:
 - ► Activate the cursor in the PC application.
 - ► Then select 🖹 or 📳 on the moisture analyzer for the relevant data output.

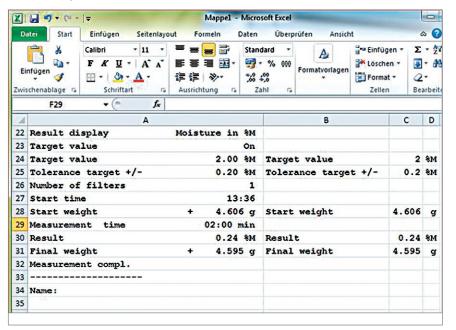

- When **PC text format** is set on the moisture analyzer, e.g., when Microsoft Word is opened:
 - ► Activate the cursor in the PC application.
 - ► Then select 🖹 or 📳 on the moisture analyzer for the relevant data output.

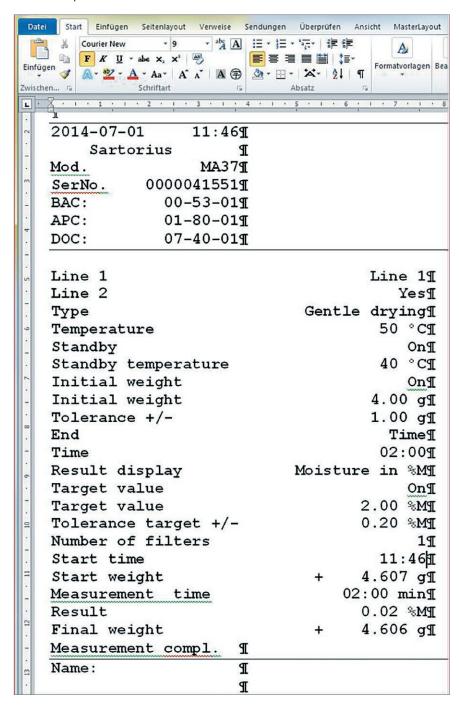


Connection with Sartorius Lab Printer YDP30, YDP40



- ► Connect the Sartorius printer with the power disconnected to the moisture analyzer via the supplied USB connection cable.
- ➤ The moisture analyzer detects the printer automatically. No settings need to be changed.

Connection for 9-pin RS-232 Configuration

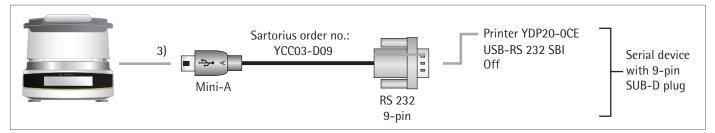

- Connect the peripheral device to the moisture analyzer using the Sartorius YCC03-D09 connection cable (RS-232, 9-pin, PC-compliant assignment).
- ► To configure the desired settings, see chapter "System Settings (Setup Menu), section "USB Port."

Interface Specification

Data Output

The print command can be triggered by selecting .

Data Output Formats

Values are always output with an ID; if more than 22 parameters are set, the values are printed on two lines. Intermediate values are also output in other formats; intermediate values are always printed on one line.

You can activate the printout in the **Printout** menu [see section "Printout" in chapter "System Settings (Setup Menu)"] and select whether values only or values and intermediate values are printed.

Example: Output of Intermediate Value 02:00 8.16% M

Output Format

The characters are printed with the header. No more than 22 characters can be displayed in one line. Longer character sets are printed out on two lines. The printout is set to justified alignment. The following characters and abbreviations are used:

Space _ A space is indicated with an underscore: _

Carriage Return CR A carriage return (or line break) is abbreviated with "CR."

Line Feed LF A line feed is abbreviated with "LF."

Example 1

The first example has a 6-character header (columns 1 to 6) and can therefore be printed in one line. Column 7 is used for signs before values (+, -). Values are given in columns 8 to 16 with decimal points or text. The unit characters are given in columns 17 to 20.

If the unit "%M/S" is selected, use four characters to print out the units because no space is printed before a unit. In a print interval, however, one line is generated with the following:

- Five characters for a header
- One character for a space
- Nine characters for the values including signs
- One space
- Four characters for the units

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22
N	_	_	_	_	_	+	_	_	_	_	6	7		8	7	_	g	_	_	C R	LF
М	0	i	s	t	_	+	_	_	_	_	_	_	_	2	2	_	%	M	_	CR	LF
1	0	:	2	3	_	+	_	_	_	_	0		2	3	_	%	M	/	S	C R	LF

Example 2

The second example has a longer header (columns 1 to 7) and can therefore be printed in one line:

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22
D	е	٧	_	_	_	+	_	_	_	5	6	7		8	7	_	g	_	_	CR	LF
S	t	а	n	d	b	у	_	_	_	_	_	_	_	_	_	0	f	f	_	CR	LF

Example 3

The third example requires more than 22 characters and must therefore be printed on two lines:

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22
R	е	s	u	ι	t	_	d	i	s	р	l	а	У	_	_	_	_	_	_	CR	LF
_	M	0	i	S	t	u	r	е	_	i	n	_	%	M	_	_	_	%	_	CR	LF

Error Messages

Certain events cause a message to appear on the display:

- 1. Some error messages are displayed for approx. 3 seconds (e.g., **CAL-Extern**: Calibration canceled).
- 2. Some error messages are displayed until they are acknowledged by a key (e.g., "Incorrect license code" for "Service access").
- 3. Information messages are displayed until they are acknowledged with a key.

Deactivated Keys

To prevent operating errors, only relevant functions/keys are displayed depending on the situation. This prevents most operating errors from occurring. The following buttons are only available in specific circumstances:

·0·	Only if there is a measured value in the zero setting range before external calibration/adjustment.
∙т∙	Only when there is a weight value larger than or smaller than "zero."
	Only if a printer is connected:

Error Messages during Operation

Display	Cause	Remedy
Err 320	Language or font files inconsistent. Not possible to load data (fonts/languages).	Contact Sartorius Service.
Err 398	The connection between internal electronic components is interrupted.	Contact Sartorius Service.
Err 401	Power input voltage too low. Supply voltage is below the lower limit.	Check voltage (see manufacturer's ID label); avoid voltage fluctuations. Contact Sartorius Service.
Err 403	Temperature sensor defective or connection to temperature sensor interrupted.	Contact Sartorius Service.
Err 404	Short circuit of temperature sensor or short circuit of the cable to the temperature sensor.	Contact Sartorius Service.
Err 406	Temporary error; max. temperature of the temperature sensor exceeded.	Disconnect the equipment from power. Allow the device to cool down. Perform a calibration/adjustment.
Err 407	Checksum error (Data flash is corrupted).	Contact Sartorius Service.

Calibration/Adjustment Error Messages

"Weight is too light."	A weight that is too light has been placed during external calibration.
"Weight is too heavy."	A weight that is too heavy has been placed during external calibration.
"Not able to save cal./adj. data."	The memory is full.

Information about Analyzer Maintenance

"Maintenance interval	The maintenance date set by the
expired"	Sartorius Service Center has been exceeded.

USB Device Error Message

"The attached USB device	A USB device (printer) that is not permitted by
is not supported."	Sartorius has been connected.

Problem

Meaning	Remedy
Selected temperature is too high and the sample is oxidized; sample is boiling or burning and the splashes are continuously changing the weight.	 Reduce drying temperature Lay glass-fiber filter onto the sample Reduce the sample quantity or apply the sample more evenly Select a semi-automatic switch-off criterion or select timer mode
Measurement time too long	 Increase temperature Reduce sample quantity Preheat the analyzer by running a drying process for 2 or 3 minutes with an empty sample pan, for example
Sample loses weight before it is analyzed	 Remove the sample pan and apply the sample outside the sample chamber
Sample is liquid or pasty	– Use glass fiber filter
Sample has only a low moisture content	– Increase sample quantity
Insufficient heating output	– Clean temperature sensor
Place of installation unstable (vibrations, etc.)	- Set up the scale in another area

Shipping the Analyzer

Please use the original packaging for shipping.


Packaging can be ordered through the Sartorius Service Center if required.




Avoid shocks and vibrations.




Prior to shipping, switch the analyzer to standby mode (see page 20) and then pull the plug.




- ► Remove the following parts from the analyzer:
 - Disposable sample pan
 - Pan support



▶ Place the analyzer in one side of the packaging.



▶ Place the other side of the packaging over the analyzer:



► Then put the packaged analyzer into the cardboard box and seal the box.

Care and Maintenance

Service

To ensure its continued weighing accuracy, we recommend performing regular servicing on your analyzer at least once a year. The Sartorius Service Center offers different service contracts for this purpose, which can be individually adapted to suit your needs (see also www.sartorius.com/service). A calibration certificate should always be issued as part of every maintenance session. The analyzer and its connections must undergo a technical safety inspection on a regular basis carried out by an electrician (e.g., every 2 years).



Repairs

Repair work must only be carried out by trained service technicians. The device must be unplugged during repair work. Unplug the power cable from the socket. Failure to do so may affect the measurement accuracy of your analyzer and pose a serious risk to the user. Contact Sartorius Service or a Sartorius dealer for proper repairs.

Cleaning the Analyzer

Cleaning the Control Panel

Switch the display to standby mode to avoid modifying the settings for operation during cleaning.



▶ Select the menu key to switch to the method menu.



▶ If you then select 🖒, the display is switched off.



► To switch the display back on: Select 🖒 at the bottom left of the display. The balance starts in the application most recently used before the it was last switched off.

Cleaning the Housing



Disconnect the analyzer from the power before cleaning. Disconnect any data cables from the moisture analyzer.



Never open the analyzer housing. The parts contained in these cannot be cleaned, repaired, or replaced by the operator.

- Make sure that no liquid or dust gets into the analyzer.
- Remove the disposable sample pan and pan support from the analyzer.
- Never use cleaning agents that contain solvents or abrasive ingredients, which can ultimately damage the equipment.
- ► Clean the outside of the housing with a lint-free cloth and mild cleaning agent (e.g., isopropanol).
- ► Then dry the analyzer with a soft cloth.



Contaminated Equipment:

- Health risk posed by product contamination due to product deposits and collection of residue with microbial contamination.
- Health risk from biological or microbiological substances.
- Observe cleaning specifications.
- Examine the cleaning results closely.

Cleaning the Heating Module




Danger of Burns:

The inner part of the heating module and parts of the sample chamber may be extremely hot.

Wait until the heating module has cooled completely.




Avoid touching the heating element. To remove spray residues or deposits from the heating element, use a weak solvent such as ethanol.




Unlocking the Heating Module

1) Open the heating module all the way.




Removing the Heating Module

2) Pull the heating module back up out of the guide.



3) Clean the heating element and temperature sensor with a weak solvent such as ethanol.




- 4) If necessary, pull the air extractor grate out of the heating module. Then clean the heating module and grate in a dishwasher.
- 5) Once cleaning is complete, reassemble the heating module and reinstall in the analyzer, following the instructions in reverse order. The heating module must snap into place on the analyzer.

Cleaning the Sample Chamber Base Plate




Danger of Burns:

Parts of the sample chamber may be extremely hot. Wait until the sample chamber base plate has cooled completely.



Removing the Sample Chamber Base Plate

1) Unlock the cover socket with a suitable coin.



- 2) Remove the cover socket and sample chamber base plate from the analyzer and clean in a dishwasher.
- 3) After cleaning, fix the sample chamber base plate into place again on the analyzer using the cover socket.

Disposal



The packaging is made of environmentally friendly materials that can be used as secondary raw materials. Packaging that is no longer needed can be disposed of in Germany free of charge via the VfW dual system (contract number D-59101-2009-1129). Otherwise, dispose of the material at your local waste management facility according to the applicable regulations. The equipment, including accessories and batteries, does not belong in your regular household waste. EU legislation requires its Member States to collect electrical and electronic equipment and dispose of it separately from other unsorted municipal waste with the aim of recycling it. For disposal or recycling, please contact our service staff on site. In addition, the partners listed on the following website are available within the EU:

- 1) Go to http://www.sartorius.com.
- Select "Services" under "Lab Products & Services."
- 3) Then select "Information on Disposal."
- 4) Addresses for local Sartorius disposal contacts can be found in the PDF files available for download on this page.



Devices contaminated with hazardous materials (NBC contamination) will not be accepted for repair or disposal.

Service Address for Disposal:

Detailed information, including service addresses for returning your device for repair or disposal, can be found on our website (www.sartorius.com) or requested from a Sartorius Service Center.

Specifications

Dryer Functions	MA37-1
Temperature range and settings	40–200°C, in increments of 1°C; stand-by temperature selectable from 50–120°C
Sample heating	Infrared heating using a metal tube heater, >480 W
Heating programs	Standard drying, gentle drying, MA35 mode
Switch-off criterion	Options: - Fully automatic - Semi-automatic mg (1–50 mg/5–300 s) - Semi-automatic &t (0.1–5.0%/5–300 s) - Time (2:00–99.59 min.) - Manual
Result display	Moisture in % M and g / dry weight in %S and g / ATRO in %M/S
Net weight, approx.	6.3 kg
Weighing Functions	
Max. weighing capacity	70 g
Repeatability, typical	Starting at an initial weight from approx. 1 g: \pm 0.2% For initial weight from approx. 5 g: \pm 0.05%
Readability	1 mg; 0.01%
Typical sample quantity	5 to 15 g
External calibration weight	50 g (E2)
Disposable sample pan dimensions	Ø 90 mm
Interface	Mini USB: Automatic detection of Sartorius printers YDP30 and YDP40, direct data transfer to Microsoft* Windows programs without additional software; programmable data output interval
Power Supply	
Input voltage	100–120 V AC and 210–240 V AC (automatic voltage detection), \pm 10%, 50/60 Hz
Protection class and standards	Protection class I as per EN 61010-1/IEC 61010-1; up to 3000 m above sea level; IP20 as per EN 60529/IEC 60529
Power supply	Using country-specific power cable from Sartorius only
Power consumption	Max. 640 W (typically)
Ambient Conditions The specifications apply under the following am	bient conditions:
Environment	For indoor use only
Ambient temperature	+10°C to +30°C
Operational capability	Operation guaranteed between +5°C and +40°C
Storage and shipping	-10°C to +60°C
Altitude	Up to 3000 m above sea level
Relative humidity	15% to 80% for temperatures up to 31°C non-condensing, decreasing linearly up to 50% relative humidity at 40°C
Safety of Electrical Equipment	In accordance with EN 61010-1/IEC 61010-1 Safety requirements for electrical equipment for measurement, control and laboratory use – Part 1: General requirements
Electromagnetic Compatibility	In accordance with EN 61326-1/IEC61326-1 Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 1: General requirements
Defined immunity to interference:	Suitable for use in industrial areas
Limitation of emissions:	Class B [suitable for use in residential areas and areas that are connected to a low voltage network that (also) supplies residential buildings]. Therefore, the analyzer can be used in both areas.


Accessories

ltem	Order No.
Disposable sample pans, 80 pcs., aluminum, \varnothing 90 mm	6965542
Glass fiber filter for analysis of pasty and fatty samples, hard quality, 80 pcs., \varnothing 90 mm	6906940
Glass fiber filter for analysis of liquid and fatty samples, soft quality, 200 pcs., \varnothing 90 mm	6906941
ReproEasy pads for the performance test, 10 pcs. to verify the repeatability of the analyzer	YHP01MA
ReproEasy pads for the performance test, 20 pcs. to verify the repeatability of the analyzer	YHP02MA
External adjustment weight: - 50 g, OIML class E2, with DKD certificate	YCW452-AC-02
Forceps	69MA0072
Printers and Communication	
Premium GLP Laboratory Printer - Printer paper for GLP lab printer - Continuous labels GLP lab printer	YDP30 69Y03285 69Y03286
Data cable for Mini USB/USB A	YCC04-D09
Data cable for Mini USB/9-pin RS-232	YCC03-D09
Data cable for Mini USB/25-pin RS-232	YCC03-D25
Spare Parts	
Protective cover for the control panel	6960SE05
Sample forceps	YST01MA

Analyzer Dimensions

MA37

All dimensions are given in millimeters

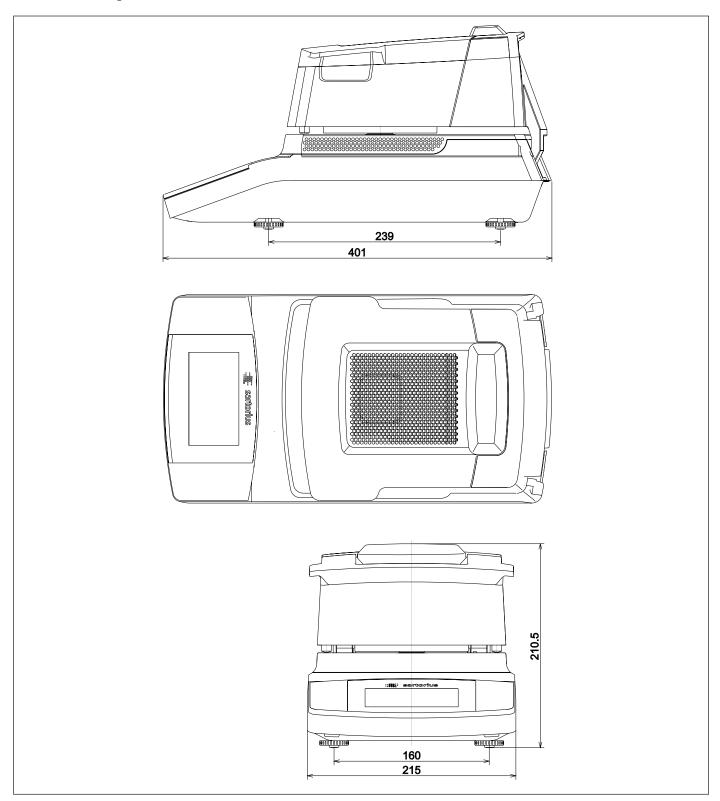





EU-Konformitätserklärung EU Declaration of Conformity

Hersteller Manufacturer Sartorius Lab Instruments GmbH & Co. KG 37070 Goettingen, Germany

erklärt in alleiniger Verantwortung, dass das Betriebsmittel declares under sole responsibility that the equipment

Geräteart Device type Feuchtebestimmer Moisture analyzer

Modell *Model* MA37-1, MA37-1CN, MA37-1US, MA37-1-CN MA160-1, MA160-1CN, MA160-1US, MA160-1-CN

in der von uns in Verkehr gebrachten Ausführung allen einschlägigen Bestimmungen der folgenden Europäischen Richtlinien – einschließlich deren zum Zeitpunkt der Erklärung geltenden Änderungen – entspricht und die anwendbaren Anforderungen folgender harmonisierter Europäischer Normen erfüllt:

in the form as delivered fulfils all the relevant provisions of the following European Directives – including any amendments valid at the time this declaration was signed – and meets the applicable requirements of the harmonized European Standards listed below:

2014/30/EU

Elektromagnetische Verträglichkeit Electromagnetic compatibility

EN 61326-1:2013

2014/35/EU

Elektrische Betriebsmittel zur Verwendung innerhalb bestimmter Spannungsgrenzen

Electrical equipment designed for use within certain voltage limits

EN 61010-1:2010

2011/65/EU

Beschränkung der Verwendung bestimmter gefährlicher Stoffe in Elektro- und Elektronikgeräten (RoHS) Restriction of the use of certain hazardous substances in electrical and electronic equipment (RoHS)

EN 50581:2012

Jahreszahl der CE-Kennzeichenvergabe / Year of the CE mark assignment: 16

Sartorius Lab Instruments GmbH & Co. KG Goettingen, 2016-09-26

Dr. Reinhard Baumfalk Vice President R&D Dr. Dieter Klausgrete

Head of International Certification Management

Diese Erklärung bescheinigt die Übereinstimmung mit den genannten EU-Richtlinien, ist jedoch keine Zusicherung von Eigenschaften. Bei einer mit uns nicht abgestimmten Änderung des Produktes verliert diese Erklärung ihre Gültigkeit. Die Sicherheitshinweise der zugehörigen Produktdokumentation sind zu beachten.

This declaration certifies conformity with the above mentioned EU Directives, but does not guarantee product attributes. Unauthorised product modifications make this declaration invalid. The safety information in the associated product documentation must be observed.

Doc: 2029910-03

SLI14CE019-03.de,en

1 / 1 PMF: 2018082

OP-113_fo1_2015.10.12

FCC Supplier's Declaration of Conformity



Device type Moisture Analyzer

Type series MA37-1US, MA160-1US

Party issuing Supplier's Declaration of Conformity / Responsible Party – U.S. Contact Information

Sartorius Corporation 5 Orville Dr Suite 200 11716 Bohemia, NY USA

Telephone: +1.631.254.4249

FCC Compliance Statement

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Information to the user

Note: This equipment has been tested and found to comply with the limits for a **class B** digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Connections between the device and peripherals must be made using shielded cables in order to maintain compliance with FCC radio frequency emission limits.

Any modifications made to this device that are not approved by Sartorius may void the authority granted to the user by the FCC to operate this equipment.

Doc: 2406962-00 SLI18FCC012-00.en 1 / 1 PMF: 2018082 OP-113_fo1_2015.10.12



Certificate of Compliance

Certificate: 70006866 Master Contract: 167555

Project: 70109280 **Date Issued:** 2017-01-16

Issued to: Sartorius Lab Instruments GmbH & Co. KG

Otto-Brenner-Strasse 20 Goettingen, 37079 GERMANY

The products listed below are eligible to bear the CSA Mark shown with adjacent indicators 'C' and 'US' for Canada and US or with adjacent indicator 'US' for US only or without either indicator for Canada only.



Issued by: Jean-Philippe Turcot Jean-Philippe Turcot

PRODUCTS

CLASS - 8721 06 - LABORATORY EQUIPMENT-Electrical

CLASS - 8721 86 - ELECTRICAL EQUIPMENT FOR LABORATORY USE-Certified to US Standards

Moisture Analyzers, Models* MA37-x-y and MA160-x-y, Rated 100-120Vac / 210-240Vac, 50/60Hz, 640W (max).

Notes*:

- 1. The above models are cord connected, Equipment Class I, Pollution Degree 2, Installation Category II.
- 2. Mode of operation: Continuous
- 3. Environmental Conditions:
 - Operating Temperature: 5 to 40°C;
 - Indoor use only;
 - Altitude: 3000 m max;
 - Relative humidity 15% to 80% for temperatures up to 31°C non-condensing, decreasing linearly up to 50% relative humidity at 40°C;
 - +/- 10% mains supply fluctuations

DQD 507 Rev. 2016-02-18

Page 1



 Certificate:
 70006866
 Master Contract:
 167555

 Project:
 70109280
 Date Issued:
 2017-01-16

- 4. The MA37 and MA160 include different models designation codes. The model designation code is MA37-x-y and MA160-x-y. Where x and y represent non safety relevant information as listed below:
 - "x" is a number (1,2,3,...) and denotes the version (e.g. 1);
 - "y" may be up to five numbers and/or letters or blank and denote special versions like country of destination, special software. The hyphens "-"may be omitted.

APPLICABLE REQUIREMENTS

CAN/CSA-C22.2 No. 61010-1-12 - Safety Requirements for Electrical Equipment for Measurement,

Control, and Laboratory Use, Part 1: General Requirements

CAN/CSA C22.2 No. 61010-2-010:15 - Particular requirements for laboratory equipment for heating of

materials

UL 61010-1 (3rd Edition) - Safety Requirements for Electrical Equipment for Measurement,

Control, and Laboratory Use - Part 1: General Requirements

UL 61010-2-010 (3rd Edition) - Particular requirements for laboratory equipment for heating of

materials

CONDITIONS OF ACCEPTABILITY

- (1) The main supply cord set provided with the equipment must be an approved type acceptable to the authorities in the country where the equipment is sold. It is the manufacturer's responsibility to provide a detachable power supply cord compliant with the requirements of sub-clause 6.10.1 and that is suitable for the country of usage and compliant to local regulations and electrical codes. A power supply cord description is provided in the List of critical components. The power supply cord shall include a protective earth wire and shall be positioning so that it cannot touch the hot surfaces of the analyzer.
- (2) <u>Intended Use:</u> The moisture analyzer can be used for determination of the moisture content of materials of liquid, pasty, and solid substances using the thermogravimetric method. The analyzer shall be use only for this purpose. Any other use outside the limits of the technical specifications is not permitted.
- (3) The analyzer must not be operated in potentially explosive atmospheres. Unit is not intended to be used with flammable liquids or materials. Materials or liquids liable to catch fire or explode shall not be used as samples for moisture analysis.
- (4) Appropriate containers must be used for each type of sample material.
- (5) If use with substances that contains poisonous or caustic ingredients, the equipment must be use under a laboratory hood.
- (6) Do not put any flammable substances on, under, or near the moisture analyzer. Minimum clearance spacing required on final installation:
 - 1 m above the analyzer
 - 20 cm around the analyzer
- (7) When operating the analyzer, suitable protective equipment must be worn in order to minimize dangers to health
- (8) Moisture analysis applications must be optimized by the user in accordance with local regulations. If at any time there is a conflict between the system safety provisions and any relevant local (national or regional) requirements, the local requirements always take precedence.

DQD 507 Rev. 2016-02-18

Page 2

Sartorius Lab Instruments GmbH & Co. KG Otto-Brenner-Strasse 20 37079 Goettingen, Germany

Phone: +49.551.308.0 www.sartorius.com

The information and figures contained in these instructions correspond to the version date specified below.

Sartorius reserves the right to make changes to the technology, features, specifications and design of the equipment without notice.

Masculine or feminine forms are used to facilitate legibility in these instructions and always simultaneously denote the other gender as well.

Copyright notice:

This instruction manual, including all of its components, is protected by copyright. Any use beyond the limits of the copyright law is not permitted without our approval. This applies in particular to reprinting, translation and editing irrespective of the type of media used.

© Sartorius Germany

Last updated: 10 | 2018

Printed in the EU on paper bleached without chlorine. | W Publication No.: WMA6068-e181009